

# Aptima® CV/TV Assay

For *in vitro* diagnostic use.  
Rx only.

<b>General Information</b>	<b>2</b>
Intended Use	2
Summary and Explanation of the Test	2
Principles of the Procedure	3
<b>Warnings and Precautions</b>	<b>3</b>
<b>Reagent Storage and Handling Requirements</b>	<b>6</b>
<b>Specimen Collection and Storage</b>	<b>7</b>
<b>Panther System</b>	<b>8</b>
Reagents and Materials Provided	8
Materials Required but Available Separately	9
<b>Panther System Test Procedure</b>	<b>10</b>
Procedural Notes	13
<b>Quality Control</b>	<b>13</b>
Assay Calibration	13
Negative and Positive Controls	13
Internal Control	14
<b>Test Interpretation</b>	<b>15</b>
<b>Limitations</b>	<b>16</b>
<b>Panther System Expected Values</b>	<b>18</b>
<b>Panther System Assay Performance</b>	<b>20</b>
Reproducibility	20
<b>Panther System Clinical Performance</b>	<b>21</b>
Performance Characteristics in Symptomatic Subjects	21
Candida Species Group Performance Characteristics	22
Candida glabrata Performance Characteristics	27
Trichomonas vaginalis Performance Characteristics	31
Positivity Rates in Asymptomatic Women	35
Invalid Rates	35
<b>Panther System Analytical Performance</b>	<b>36</b>
Analytical Sensitivity	36
Analytical Inclusivity	36
Cross-Reactivity and Microbial Interference	37
Interference	38
Within Laboratory Precision	39
Co-Infection	40
<b>Bibliography</b>	<b>41</b>

## General Information

### Intended Use

The Aptima® CV/TV assay is an *in vitro* nucleic acid amplification test for the detection of RNA from microorganisms associated with vulvovaginal candidiasis and trichomoniasis. The assay utilizes real time transcription-mediated amplification (TMA) to detect and qualitatively report results for the following organisms:

- *Candida* species group (*C. albicans*, *C. tropicalis*, *C. parapsilosis*, *C. dubliniensis*)
- *Candida glabrata*
- *Trichomonas vaginalis*

The assay differentiates between *Candida glabrata* and the *Candida* species group (C spp) by targeting the RNA component of RNase P ribonucleoprotein; the assay does not differentiate among C spp. For *Trichomonas vaginalis*, the assay targets ribosomal RNA (rRNA) and differentiates the result from results for *Candida glabrata* and C spp. The assay is intended to aid in the diagnosis of vulvovaginal candidiasis and trichomoniasis on the automated Panther® system using clinician-collected and patient-collected vaginal swab specimens from females with a clinical presentation consistent with vaginitis or vulvovaginitis.

### Summary and Explanation of the Test

Vaginitis syndrome is characterized by a spectrum of conditions; vaginal and vulvar irritation, odor, discharge and pruritus (1). Causes of vaginitis include mechanical and chemical factors (feminine hygiene products, contraceptive materials, etc.) as well as infectious agents (1). Up to 90% of infectious vaginitis cases are caused by bacterial vaginosis (BV), vulvovaginal candidiasis (candida vaginitis, CV) and trichomoniasis (*Trichomonas vaginalis*, TV) (2). BV has been diagnosed in 22-50% of symptomatic patients, CV in 17-39%, and TV in 4-35% (1,2).

CV, commonly known as a yeast infection, is the second and most frequent cause of vaginitis. CV is characterized by an overgrowth of *Candida* species in the vaginal tract and is associated with clinical signs of inflammation (3). Up to 89% of CV cases are caused by *C. albicans*, while non-*albicans* species may be responsible for 11% (3). Characteristic symptoms for CV include abnormal vaginal discharge, vaginal soreness, pruritus, dyspareunia, and external dysuria (4). *C. glabrata*, which is responsible for the majority of non-*albicans* CV in the U.S., may have decreased susceptibility to standard antimycotic therapeutic intervention compared to *C. albicans* (4,5). *C. glabrata* infections therefore require special attention in clinical management.

TV is the third most common cause of infectious vaginitis (2). The causative agent, the protozoan parasite TV, is transmitted by unprotected penile-vaginal sex (4). Women infected with TV during pregnancy have increased risk for adverse pregnancy outcomes, such as premature rupture of membranes, preterm delivery, and low birth weight (4). TV infection is associated with an increased risk of HIV acquisition and transmission (6,7), as well as prolonged HPV infection (11) and concurrent sexually transmitted infections (chlamydia, gonorrhea, and herpes simplex virus types 1 & 2) (12).

CV and TV may be detected by microscopy, culture, and nucleic acid using specimens collected with vaginal swabs.

The Aptima CV/TV assay is a real time TMA assay developed for use on the automated Panther system that detects and discriminates RNA markers from C spp, *C. glabrata*, and TV

in clinician-collected and patient-collected vaginal swab specimens from symptomatic females. The Aptima CV/TV assay includes an internal control (IC).

## Principles of the Procedure

The Aptima CV/TV assay involves three main steps, all of which take place in a single tube on the Panther system: target capture, target amplification by TMA, and detection of the amplification products (amplicon) by fluorescent labeled probes (torches). The assay incorporates an internal control (IC) in every test to monitor nucleic acid capture, amplification, and detection.

Specimens are collected in a tube containing specimen transport media (STM) that lyses the organisms, releases the RNA, and protects it from degradation during storage. When the assay is performed, capture oligonucleotides hybridize to highly conserved regions of the target RNA, if present, in the test specimen. The hybridized target is then captured onto magnetic microparticles that are separated from the specimen in a magnetic field. Wash steps remove extraneous components from the reaction tube.

Target amplification occurs via TMA, a transcription-based nucleic acid amplification method that utilizes two enzymes, Moloney murine leukemia virus (MMLV) reverse transcriptase and T7 RNA polymerase. The reverse transcriptase is used to generate a DNA copy of the target RNA sequence, adding a promoter sequence for T7 RNA polymerase. T7 RNA polymerase produces multiple copies of RNA amplicon from the DNA copy template.

Detection is achieved using single-stranded nucleic acid torches that are present during the amplification of the target and hybridize specifically to the amplicon in real time. Each torch has a fluorophore and a quencher. The quencher suppresses the fluorescence of the fluorophore when the torch is not hybridized to the amplicon. When the torch binds to the amplicon, the fluorophore is separated from the quencher and emits a signal at a specific wavelength when excited by a light source. The Panther system detects and discriminates between four fluorescent signals corresponding to C spp, *C. glabrata*, TV, and IC amplification products. The Panther system software uses an Aptima CV/TV assay-specific algorithm that interprets the amplification signal emergence times to generate a Positive or Negative status for each target organism in the sample.

## Warnings and Precautions

- A. For *in vitro* diagnostic use.
- B. To reduce the risk of invalid results, carefully read the entire package insert and the *Panther System Operator's Manual* prior to performing this assay.
- C. Only personnel adequately trained in the use of the Aptima CV/TV assay and in handling potentially infectious materials should perform this procedure. If a spill occurs, immediately disinfect following appropriate site procedures.
- D. For additional specific warnings and precautions, refer to the *Panther System Operator's Manual*.

## Laboratory Related

- E. Use only supplied or specified disposable laboratory ware.

- F. Use routine laboratory precautions. Do not pipette by mouth. Do not eat, drink or smoke in designated work areas. Wear disposable, powderless gloves, protective eye wear, and laboratory coats when handling specimens and kit reagents. Wash hands thoroughly after handling specimens and kit reagents.
- G. Work surfaces, pipettes, and other equipment must be regularly decontaminated with 2.5% to 3.5% (0.35 M to 0.5 M) sodium hypochlorite solution. Thoroughly clean and disinfect all work surfaces.
- H. Dispose of all materials that have come in contact with specimens and reagents in accordance with applicable national, international, and regional regulations (8, 9, 10). Thoroughly clean and disinfect all work surfaces.

### Specimen Related

- I. Expiration dates for the collection kits pertain to the collection of specimens and not to the specimen testing. Samples collected any time prior to the expiration date of the collection kit, and transported and stored in accordance with the package insert, are valid for testing even if the expiration date on the collection tube has passed.
- J. Specimens may be infectious. Use Universal Precautions when performing this assay (8, 9). Proper handling and disposal methods should be established according to local regulations (10). Only personnel adequately trained in the use of the Aptima CV/TV assay and trained in handling infectious materials should perform this procedure.
- K. Maintain proper storage conditions during specimen shipping to ensure the integrity of the specimen. Specimen stability under shipping conditions other than those recommended has not been evaluated.
- L. Avoid cross-contamination during the specimen handling steps. Specimens can contain extremely high levels of organisms. Ensure that specimen containers do not contact one another, and discard used materials without passing over any open container. Change gloves if they come in contact with a specimen.
- M. Upon piercing, liquid can discharge from Aptima transfer tube caps under certain conditions. Refer to the *Panther System Test Procedure* for more information.
- N. If the lab receives an Aptima Multitest Swab Specimen Collection Kit transport tube with no swab, two swabs, a cleaning swab, or a swab not supplied by Hologic, the specimen must be rejected.

### Assay Related

- O. Do not interchange, mix, or combine assay reagents from kits with different master lot numbers. Controls, the calibrator, and assay fluids may be interchanged.
- P. Cap and store reagents at the specified temperatures. The performance of the assay may be affected by use of improperly stored reagents. See *Reagent Storage and Handling Requirements* and *Panther System Test Procedure* for more information.
- Q. Do not combine any assay reagents or fluids without specific instruction. Do not top off reagents or fluids. The Panther system verifies reagent levels.

- R. Avoid microbial and nuclease contamination of reagents.
- S. Do not use the reagent, control, or calibrator kits after the expiration date.
- T. Some reagents used with the Aptima CV/TV assay are labeled with risk and safety symbols.

**Note:** Hazard Communication information for labeling of globally marketed products reflects the US and EU Safety Data Sheets (SDS) classifications. For hazard communication information specific to your region, refer to the region specific SDS on the Safety Data Sheet Library at [www.hologicsds.com](http://www.hologicsds.com).

US Hazard Information
<b>Target Capture Reagent</b> <b>EDTA 1-5%</b> <b>LITHIUM HYDROXIDE, MONOHYDRATE 1-5%</b> H412 - Harmful to aquatic life with long lasting effects. H401 - Toxic to aquatic life.
EU Hazard Information
<b>Target Capture Reagent</b> <b>EDTA 1-5%</b> <b>LITHIUM HYDROXIDE, MONOHYDRATE 1-5%</b> H412 - Harmful to aquatic life with long lasting effects. P273 - Avoid release to the environment P280 - Wear eye protection/ face protection


## Reagent Storage and Handling Requirements

- A. The following table shows the storage conditions and stability for the reagents, the calibrator, and the controls.

Reagent	Unopened Storage	Open Kit (Reconstituted)	
		Storage	Stability
Amplification Reagent	2°C to 8°C		
Amplification Reconstitution Solution	15°C to 30°C	2°C to 8°C	30 days <sup>1</sup>
Enzyme Reagent	2°C to 8°C		
Enzyme Reconstitution Solution	15°C to 30°C	2°C to 8°C	30 days <sup>1</sup>
Promoter Reagent	2°C to 8°C		
Promoter Reconstitution Solution	15°C to 30°C	2°C to 8°C	30 days <sup>1</sup>
Target Capture Reagent	15°C to 30°C	15°C to 30°C <sup>2</sup>	30 days <sup>1</sup>
Positive Calibrator	2°C to 8°C		Single use vial
Negative Control	2°C to 8°C		Single use vial
Positive Control	2°C to 8°C		Single use vial
Internal Control	2°C to 8°C		Single use vial

<sup>1</sup> When reagents are removed from the Panther system, they should be immediately returned to their appropriate storage temperatures.

<sup>2</sup> Storage condition for the working Target Capture Reagent (Target Capture Reagent with Internal Control added).

- B. Discard any unused reconstituted reagents and working Target Capture Reagent (wTCR) after 30 days or after the Master Lot expiration date, whichever comes first.
- C. Reagents stored on the Panther system have 120 hours of onboard stability. Reagents can be loaded onto the Panther system up to 5 times. The system logs each time the reagents are loaded.
- D.  The Promoter Reagent and reconstituted Promoter Reagent are photosensitive. Protect these reagents from light during storage and preparation for use.
- E. Avoid cross-contamination during reagent handling and storage. Recap all reconstituted reagents with new reagent caps prior to storage.
- F. **Do not freeze reagents.**

## Specimen Collection and Storage

**Note:** Handle all specimens as if they contain potentially infectious agents. Use Universal Precautions.

**Note:** Take care to avoid cross-contamination during sample handling steps. For example, discard used material without passing over open tubes.

Vaginal swab specimens can be tested with the Aptima CV/TV assay. Assay performance has not been evaluated with specimens other than those collected with the following specimen collection kit:

- Aptima Multitest Swab Specimen Collection Kit

### A. Specimen collection

Refer to the appropriate specimen collection kit package insert for specific collection instructions.

### B. Specimen transport and storage before testing:

#### 1. Swab specimens

- a. After collection, swab specimens in transport tubes can be stored at 2°C to 30°C for up to 30 days.
- b. If longer storage is needed, swab specimens in transport tubes can be stored at -20°C or -70°C for an additional 60 days.

### C. Specimen storage after testing:

1. Specimens that have been assayed must be stored upright in a rack.
2. The specimen transport tubes should be covered with a new, clean plastic film or foil barrier.
3. If assayed samples need to be shipped, remove penetrable cap and place new non-penetrable caps on the specimen transport tubes. If specimens need to be shipped for testing at another facility, recommended temperatures should be maintained.
4. Prior to uncapping, specimen transport tubes must be centrifuged for 5 minutes at  $420 \pm 100$  relative centrifugal force (RCF) to bring all of the liquid down to the bottom of the tube. **Avoid splashing and cross-contamination.**

**Note:** Specimens must be shipped in accordance with applicable national, international, and regional transportation regulations.

## Panther System

Reagents for the Aptima CV/TV assay are listed below for the Panther system. Reagent Identification Symbols are also listed next to the reagent name.

### Reagents and Materials Provided

**Note:** For information on any hazard and precautionary statements that may be associated with reagents, refer to the Safety Data Sheet Library at [www.hologic.com/sds](http://www.hologic.com/sds).

#### Aptima CV/TV Assay Kit

100 tests: 2 assay boxes, 1 calibrator kit, and 1 controls kit (Cat. No. PRD-05189)

#### Aptima CV/TV Assay Refrigerated Box (store at 2°C to 8°C upon receipt)

Symbol	Component	Quantity
<b>A</b>	<b>Amplification Reagent</b> <i>Non-infectious nucleic acids dried in buffered solution.</i>	1 vial
<b>E</b>	<b>Enzyme Reagent</b> <i>Reverse transcriptase and RNA polymerase dried in HEPES buffered solution.</i>	1 vial
<b>PRO</b>	<b>Promoter Reagent</b> <i>Non-infectious nucleic acids dried in buffered solution.</i>	1 vial
<b>IC</b>	<b>Internal Control</b> <i>Non-infectious nucleic acids in buffered solution.</i>	1 x 0.3 mL

#### Aptima CV/TV Assay Room Temperature Box (store at 15°C to 30°C upon receipt)

Symbol	Component	Quantity
<b>AR</b>	<b>Amplification Reconstitution Solution</b> <i>Aqueous solution containing glycerol and preservatives.</i>	1 x 7.2 mL
<b>ER</b>	<b>Enzyme Reconstitution Solution</b> <i>HEPES buffered solution containing a surfactant and glycerol.</i>	1 x 5.8 mL
<b>PROR</b>	<b>Promoter Reconstitution Solution</b> <i>Aqueous solution containing glycerol and preservatives.</i>	1 x 4.5 mL
<b>TCR</b>	<b>Target Capture Reagent</b> <i>Buffered salt solution containing non-infectious nucleic acids and magnetic particles.</i>	1 x 26.0 mL
	<b>Reconstitution Collars</b>	3
	<b>Master Lot Barcode Sheet</b>	1 sheet



**Aptima CV/TV Assay Calibrator Kit (PRD-05191)**  
(store at 2°C to 8°C upon receipt)

Symbol	Component	Quantity
PCAL	<b>Positive Calibrator</b> <i>Non-infectious nucleic acids in buffered solution.</i>	5 x 2.8 mL
	<b>Calibrator Barcode Label</b>	1 sheet

**Aptima CV/TV Assay Controls Kit (PRD-05190)**  
(store at 2°C to 8°C upon receipt)

Symbol	Component	Quantity
CONTROL-	<b>Negative Control</b> <i>Buffered solution.</i>	5 x 2.7 mL
CONTROL+	<b>Positive Control</b> <i>Non-infectious C. albicans, C. glabrata, and T. vaginalis cultured organisms in buffered solution.</i>	5 x 1.7 mL
	<b>Control Barcode Label</b>	1 sheet

### Materials Required but Available Separately

*Note: Materials available from Hologic have catalog numbers listed, unless otherwise specified.*

Material	Cat. No.
Panther System	-
Panther Run Kit for Real Time Assays (for real time assays only)	PRD-03455 (5000 tests)
<i>Aptima Assay Fluids Kit (also known as Universal Fluids Kit) Contains Aptima Wash Solution, Aptima Buffer for Deactivation Fluid, and Aptima Oil Reagent</i>	303014 (1000 tests)
<i>Multi-tube units (MTUs)</i>	104772-02
<i>Panther Waste Bag Kit</i>	902731
<i>Panther Waste Bin Cover</i>	504405
Or, Panther System Run Kit	303096 (5000 tests)
<i>When running non-real time-TMA assays in parallel with real time-TMA assays Contains MTUs, waste bags, waste bin covers, auto detect, and assay fluids</i>	
Aptima Assay Fluids Kit	303014 (1000 tests)
<i>Contains Aptima Wash Solution, Aptima Buffer for Deactivation Fluid, and Aptima Oil Reagent</i>	
Multi-tube units (MTUs)	104772-02
Tips, 1000 µL conductive, liquid sensing	10612513 (Tecan)
Aptima Multitest Swab Specimen Collection Kit	PRD-03546
Bleach, 5.0% to 7.0% (0.7 M to 1.0 M) sodium hypochlorite solution	--

Material	Cat. No.
Disposable, powderless gloves	--
Aptima penetrable caps	105668
Replacement non-penetrable caps	103036A
Reagent Replacement Caps	
<i>Amplification, Enzyme, and Promoter reagent reconstitution bottles</i>	CL0041 (100 caps)
<i>TCR bottle</i>	501604 (100 caps)
Plastic-backed laboratory bench covers	--
Lint-free wipes	--
Pipettor	--
Tips	--
Tube Rocker	--

## Panther System Test Procedure

**Note:** See the Panther System Operator's Manual for additional Panther system procedural information.

### A. Work Area Preparation

1. Clean work surfaces where reagents will be prepared. Wipe down work surfaces with 2.5% to 3.5% (0.35 M to 0.5 M) sodium hypochlorite solution. Allow the sodium hypochlorite solution to contact surfaces for at least 1 minute and then follow with a deionized (DI) water rinse. Do not allow the sodium hypochlorite solution to dry.
2. Clean a separate work surface where samples will be prepared. Use the procedure described above (Step A.1).
3. Cover the bench surfaces on which the reagents and samples will be prepared with clean, plastic-backed absorbent laboratory bench covers.
4. Wipe pipettors with 2.5% to 3.5% (0.35 M to 0.5 M) sodium hypochlorite solution. Allow the sodium hypochlorite solution to contact surfaces for at least 1 minute and then follow with a DI water rinse. Do not allow the sodium hypochlorite solution to dry.

### B. Reagent Reconstitution/Preparation of a New Kit


**Note:** Reagent reconstitution should be performed prior to beginning any work on the Panther system.

1. Prior to testing, Amplification, Enzyme, and Promoter Reagents must be reconstituted by combining contents of the bottles of lyophilized reagent with the appropriate reconstitution solution.
  - a. Allow the lyophilized reagents to reach room temperature (15°C to 30°C) before use.
  - b. Pair each reconstitution solution with its lyophilized reagent. Before attaching the reconstitution collar, ensure that the reconstitution solution and reagent have matching label symbols.

- c. Check the lot numbers on the Master Lot Barcode Sheet to ensure that the appropriate reagents are paired.
- d. Open the lyophilized reagent vial and firmly insert the notched end of the reconstitution collar into the vial opening (Figure 1, Step 1).
- e. Open the matching reconstitution solution bottle, and set the cap on a clean, covered work surface.
- f. While holding the reconstitution solution bottle on the bench, firmly insert the other end of the reconstitution collar into the bottle opening (Figure 1, Step 2).
- g. Slowly invert the assembled bottles. Allow the solution to drain from the bottle into the glass vial (Figure 1, Step 3).
- h. Gently swirl the solution in the bottle to mix. Avoid creating foam while swirling the bottle (Figure 1, Step 4).
- i. Wait at least 15 minutes for the lyophilized reagent to go into solution, then invert the assembled bottles again, tilting at a 45° angle to minimize foaming (Figure 1, Step 5). Allow all of the liquid to drain back into the plastic bottle.
- j. Remove the reconstitution collar and glass vial (Figure 1, Step 6).
- k. Recap the plastic bottle. Record operator initials and reconstitution date on the label (Figure 1, Step 7).
- l. Discard the reconstitution collar and glass vial (Figure 1, Step 8).

**Option:** Additional mixing of the Amplification, Enzyme, and Promoter Reagents using a tube rocker is allowed. The reagents may be mixed by placing the recapped plastic bottle on a tube rocker set to 20 RPM (or equivalent) for a minimum of 5 minutes.

**Warning:** Avoid creating foam when reconstituting reagents. Foam compromises the level-sensing in the Panther system.

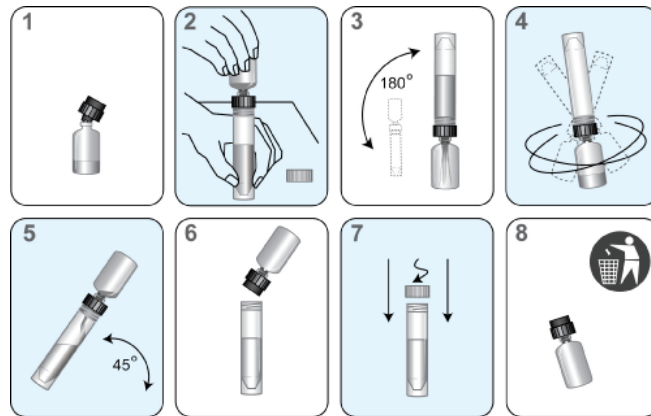

**Figure 1. Reagent Reconstitution Process**

2. Prepare Working Target Capture Reagent (wTCR)
  - a. Pair the appropriate bottles of TCR and IC.
  - b. Check the reagent lot numbers on the Master Lot Barcode Sheet to make sure that the appropriate reagents in the kit are paired.
  - c. Open the bottle of TCR, and set the cap on a clean, covered work surface.

- d. Open the bottle of IC and pour the entire contents into the bottle of TCR. Expect a small amount of liquid to remain in the IC bottle.
- e. Cap the bottle and gently swirl the solution to mix the contents. Avoid creating foam during this step.
- f. Record operator initials and the current date on the label.
- g. Discard the IC bottle and cap.

#### C. Reagent Preparation for Previously Prepared Reagents

1. Previously prepared Amplification, Enzyme, and Promoter reagents must reach room temperature (15°C to 30°C) prior to the start of the assay.

**Option:** The reagents may be brought to room temperature by placing the reconstituted Amplification, Enzyme, and Promoter Reagents on a tube rocker set to 20 RPM (or equivalent) for a minimum of 25 minutes.

2. If wTCR contains precipitate, warm wTCR at 42°C to 60°C for up to 90 minutes. Allow the wTCR to equilibrate to room temperature prior to use. Do not use if precipitate persists.
3. Verify that the reagents have not exceeded their storage stability times, including onboard stability.
4. Thoroughly mix each reagent by gently inverting prior to loading on the system. Avoid creating foam when inverting reagents.
5. Do not top off reagent bottles. The Panther system will recognize and reject bottles that have been topped off.

#### D. Specimen Handling

1. Allow the controls and specimens to reach room temperature prior to processing.
2. **Do not vortex specimens.**
3. Visually confirm that each specimen tube meets the following criteria:
  - a. The presence of a single pink Aptima collection swab in a swab specimen transport tube.
4. Inspect specimen tubes before loading into rack:
  - a. If a specimen tube contains bubbles in the space between the liquid and the cap, centrifuge the tube for 5 minutes at 420 RCF to eliminate the bubbles.
  - b. If a specimen tube has a lower volume than typically observed when collection instructions have been followed, centrifuge the tube for 5 minutes at 420 RCF to ensure that no liquid is in the cap.

**Note:** Failure to follow Steps 4a-4b may result in liquid discharge from the specimen tube cap.

**Note:** Up to 4 separate aliquots can be tested from each specimen tube. Attempts to pipette more than 4 aliquots from the specimen tube can lead to processing errors.

#### E. System Preparation

1. Set up the system according to the instructions in the *Panther System Operator's Manual* and *Procedural Notes*. Make sure that the appropriately sized reagent racks and TCR adapters are used.

## Procedural Notes

### A. Calibrator and Controls

Allow the calibrator and controls to reach room temperature prior to processing.

1. The positive calibrator, positive control and negative control tubes can be loaded in any rack position or in any Sample Bay Lane on the Panther system. Specimen pipetting will begin when one of the following 2 conditions has been met:
  - a. The calibrator and controls are currently being processed by the system.
  - b. Valid results for the calibrator and controls are registered on the system.
2. Once the calibrator and control tubes have been pipetted and are processing for a specific reagent kit, patient specimens can be tested with the associated kit up to 24 hours **unless**:
  - a. The calibrator result or control results are invalid.
  - b. The associated assay reagent kit is removed from the system.
  - c. The associated assay reagent kit has exceeded stability limits.
3. Each calibrator or each control tube can be used once. Attempts to use more than once can lead to processing errors.

### B. Temperature

Room temperature is defined as 15°C to 30°C.

### C. Glove Powder

As in any reagent system, excess powder on some gloves may cause contamination of opened tubes. Powderless gloves are recommended.

## Quality Control

An operator may invalidate an individual specimen or an entire run if it was observed and documented that a procedural, technical, or instrument-related error occurred while performing the assay.

## Assay Calibration

To generate valid results, an assay calibration must be completed. The calibrator is run in triplicate each time a reagent kit is loaded on the Panther system. Once established, the calibration is valid for up to 24 hours. Software on the Panther system alerts the operator when a calibration is required. The operator scans the calibration coefficients found on the Master Lot Barcode Sheet provided with each reagent kit.

During processing, criteria for acceptance of the calibrator is automatically verified by the software on the Panther system. If less than two of the calibrator replicates are valid, the software automatically invalidates the run. Samples in an invalidated run must be retested using a freshly prepared calibrator and freshly prepared controls.

## Negative and Positive Controls

To generate valid results, a set of assay controls must be tested. One replicate each of the negative control and positive control must be tested each time a reagent kit is loaded on the

Panther system. Once established, the controls are valid for up to 24 hours. Software on the Panther system alerts the operator when controls are required.

During processing, criteria for acceptance of controls are automatically verified by software on the Panther system. If any one of the controls has an invalid result, the software automatically invalidates the run. Samples in an invalidated run must be retested using a freshly prepared calibrator and freshly prepared controls.

### **Internal Control**

Each sample contains an IC. During processing, IC acceptance criteria are automatically verified by the Panther system software. If an IC result is invalid, the sample result is invalidated. Every sample with an invalid IC result must be retested to obtain a valid result.

The Panther system software is designed to accurately verify processes when procedures are performed following the instructions provided in this package insert and the *Panther System Operator's Manual*.

## Test Interpretation

Test results are automatically determined by the assay software. Results for CV/TV detection are reported separately. The table below shows the possible results reported in a valid run and result interpretations. Samples with invalid test results should be retested.

Table 1: *Result Interpretation*

<b>C spp Result</b>	<b><i>C. glabrata</i> Result</b>	<b>TV Result</b>	<b>Result</b>	<b>Interpretation</b>
Positive	Negative	Negative	Valid	<i>Candida</i> species group RNA detected.
Positive	Positive	Negative	Valid	<i>Candida</i> species group RNA and <i>Candida glabrata</i> RNA detected.
Positive	Negative	Positive	Valid	<i>Candida</i> species group RNA and <i>Trichomonas vaginalis</i> RNA detected.
Positive	Positive	Positive	Valid	<i>Candida</i> species group RNA, <i>Candida glabrata</i> RNA, and <i>Trichomonas vaginalis</i> RNA detected.
Negative	Positive	Negative	Valid	<i>Candida glabrata</i> RNA detected.
Negative	Negative	Positive	Valid	<i>Trichomonas vaginalis</i> RNA detected.
Negative	Positive	Positive	Valid	<i>Candida glabrata</i> RNA and <i>Trichomonas vaginalis</i> RNA detected.
Negative	Negative	Negative	Valid	Negative for <i>Candida</i> species group, <i>Candida glabrata</i> and <i>Trichomonas vaginalis</i> .
Invalid	Invalid	Invalid	Invalid	Invalid: there was an error in the generation of the result. Specimen should be retested.

Note: *Candida* species group RNA=*C. albicans*, *C. parapsilosis*, *C. dubliniensis*, and/or *C. tropicalis*

## Limitations

- A. Use of this assay is limited to personnel who have been trained in the procedure. Failure to follow the instructions given in this package insert may result in erroneous results.
- B. The effects of tampon use, douching, and specimen collection variables have not been evaluated for their impact on assay performance.
- C. Performance with specimen types other than vaginal swab specimens has not been evaluated.
- D. Reliable results are dependent on adequate specimen collection, transport, storage, and processing. Because the transport system used for this assay does not permit microscopic assessment of specimen adequacy, proper specimen collection techniques are necessary. See *Specimen Collection and Storage* for instructions. For detailed information, refer to the appropriate instructions for use.
- E. Therapeutic failure or success cannot be determined with the Aptima CV/TV assay since nucleic acid may persist following appropriate antimicrobial therapy.
- F. Results from the Aptima CV/TV assay should be interpreted in conjunction with other clinical data available to the clinician.
- G. A negative result does not preclude a possible infection because results are dependent on adequate specimen collection. Test results may be affected by improper specimen collection, technical error, specimen mix-up, or target levels below the assay limit of detection (LoD).
- H. The Aptima CV/TV assay provides qualitative results. Therefore, a correlation cannot be drawn between the magnitude of a positive assay signal and the number of organisms in a specimen.
- I. Performance of the assay has not been evaluated in women less than 14 years of age.
- J. Customers must independently validate an LIS transfer process.
- K. The Aptima CV/TV assay has not been evaluated for use with specimens collected by patients at home.
- L. Collection and testing of patient-collected vaginal swab specimens with the Aptima CV/TV assay is not intended to replace clinical examination. Vaginal infections may result from other causes or concurrent infections may occur.
- M. A *Candida* species group positive result can be due to one or multiple *Candida* species.
- N. Interference with the Aptima CV/TV assay was observed in the presence of the following substances: Tioconazole 6.5% Ointment (3% W/V, all analytes), Vaginal Moisturizing Gel (1% W/V, C spp; 5% W/V, *C. glabrata*; 3% W/V, TV), and Glacial Acetic Acid (5% V/V, C spp only).



- O. The following organism was observed to cross-react above the stated concentrations:  
*Candida famata* at concentrations higher than  $5 \times 10^5$  CFU/mL.
- P. Competitive interference was observed in co-infected samples for the combination of low *C. glabrata* (3X LoD) and high *T. vaginalis* ( $1 \times 10^5$  or  $1 \times 10^4$  cells/mL).
- Q. A positive test result does not necessarily indicate the presence of viable organisms. A positive result is indicative of the presence of target RNA.

## Panther System Expected Values

The prevalence of *Candida* and *T. vaginalis* in patient populations depends on age, race/ethnicity, risk factors, the type of clinic, and the sensitivity of the test used to detect infections. A summary of the positivity of *Candida* species group, *C. glabrata*, and *T. vaginalis* detection in symptomatic subjects, as determined by the Aptima CV/TV assay on the Panther system, is shown in Table 2 for the multi-center study, by clinical site and overall.

Table 2: Positivity as Determined by the Aptima CV/TV Assay in Symptomatic Women by Specimen Type and Clinical Site

% Positivity (# positive/# tested with valid results)						
Site	Clinician-collected Vaginal Swabs			Patient-collected Vaginal Swabs		
	<i>Candida</i> species group <sup>1</sup>	<i>C. glabrata</i>	<i>T. vaginalis</i>	<i>Candida</i> species group <sup>1</sup>	<i>C. glabrata</i>	<i>T. vaginalis</i>
1	15.0 (3/20)	5.0 (1/20)	6.3 (1/16)	20.0 (4/20)	5.0 (1/20)	6.3 (1/16)
2	20.0 (1/5)	0.0 (0/5)	0.0 (0/1)	0.0 (0/5)	0.0 (0/5)	0.0 (0/1)
3	54.5 (12/22)	0.0 (0/22)	9.5 (2/21)	54.5 (12/22)	0.0 (0/22)	9.5 (2/21)
4	23.1 (50/216)	5.1 (11/216)	30.5 (65/213)	28.2 (60/213)	7.0 (15/213)	18.0 (38/211)
5	25.9 (38/147)	4.8 (7/146)	9.0 (13/145)	28.5 (41/144)	5.6 (8/144)	7.7 (11/143)
6	33.3 (24/72)	4.2 (3/72)	2.9 (2/68)	33.3 (24/72)	4.2 (3/72)	1.5 (1/68)
7	24.4 (48/197)	7.6 (15/197)	36.5 (72/197)	27.9 (55/197)	7.1 (14/197)	28.9 (57/197)
8	0.0 (0/1)	0.0 (0/1)	100.0 (1/1)	0.0 (0/1)	0.0 (0/1)	100.0 (1/1)
9	38.0 (41/108)	1.9 (2/108)	3.8 (4/105)	46.3 (50/108)	2.8 (3/108)	3.8 (4/105)
10	47.1 (8/17)	5.9 (1/17)	0.0 (0/17)	52.9 (9/17)	5.9 (1/17)	0.0 (0/17)
11	26.8 (19/71)	5.6 (4/71)	11.4 (8/70)	27.8 (20/72)	5.6 (4/72)	5.6 (4/71)
12	33.3 (46/138)	2.9 (4/138)	2.3 (3/130)	34.1 (46/135)	3.0 (4/135)	2.3 (3/129)
13	30.4 (21/69)	1.4 (1/69)	13.0 (9/69)	31.9 (22/69)	2.9 (2/68)	11.6 (8/69)
14	44.4 (4/9)	0.0 (0/9)	0.0 (0/8)	44.4 (4/9)	0.0 (0/9)	0.0 (0/8)
15	50.0 (2/4)	0.0 (0/4)	0.0 (0/4)	50.0 (2/4)	0.0 (0/4)	0.0 (0/4)
16	40.0 (12/30)	3.3 (1/30)	10.7 (3/28)	46.7 (14/30)	3.3 (1/30)	10.7 (3/28)
17	37.5 (30/80)	2.5 (2/80)	2.7 (2/74)	40.0 (32/80)	1.3 (1/80)	4.1 (3/74)
18	36.0 (31/86)	1.2 (1/85)	4.8 (4/83)	37.2 (32/86)	1.2 (1/85)	4.8 (4/83)
19	44.0 (33/75)	5.3 (4/75)	2.8 (2/71)	48.0 (36/75)	5.3 (4/75)	2.8 (2/71)

Table 2: Positivity as Determined by the Aptima CV/TV Assay in Symptomatic Women by Specimen Type and Clinical Site

% Positivity (# positive/# tested with valid results)						
	Clinician-collected Vaginal Swabs			Patient-collected Vaginal Swabs		
20	10.3 (4/39)	5.1 (2/39)	0.0 (0/39)	10.3 (4/39)	5.1 (2/39)	0.0 (0/39)
21	20.3 (16/79)	5.1 (4/79)	11.5 (9/78)	25.3 (20/79)	5.1 (4/79)	10.4 (8/77)
All	29.8 (443/1485)	4.2 (63/1483)	13.9 (200/1438)	33.0 (487/1477)	4.6 (68/1475)	10.5 (150/1433)

<sup>1</sup> *Candida albicans*, *Candida tropicalis*, *Candida parapsilosis*, and/or *Candida dubliniensis*.

## Panther System Assay Performance

### Reproducibility

Aptima CV/TV assay reproducibility was evaluated on the Panther system at three US sites using seven panel members. Two operators performed testing at each site. Each operator performed one run per day over six days using one reagent lot over the course of testing. Each run had three replicates of each panel member.

The panel members were made using a simulated vaginal swab matrix ('SVSM', which contains specimen transport media (STM) spiked with simulated vaginal fluid) negative for *Candida* species and *T. vaginalis*. Six positive panel members were created by spiking the SVSM matrix with approximately 2X C<sub>95</sub> or LoD (low-positive) or 3X C<sub>95</sub> or LoD (moderate positive) concentrations of whole cell lysates positive for *C. albicans*, *C. glabrata*, or *T. vaginalis*. One negative panel member contained only the matrix with no added target analytes.

The agreement with expected results was 100% for all panel members.

Signal variability of the Aptima CV/TV assay was calculated for each target in analyte positive panel members. Only samples with valid results were included in the analyses. Variability, calculated between sites, between operators, between days, between runs, within runs, and overall, is shown in Table 3.

Table 3: Signal Variability by Positive Panel Members

Panel Description	N	Mean TTime <sup>1</sup>	Between Sites		Between Operators		Between Days		Between Runs		Within Runs		Total	
			SD	CV (%)	SD	CV (%)	SD	CV (%)	SD	CV (%)	SD	CV (%)	SD	CV (%)
<i>C. albicans</i> Low Pos <sup>1</sup>	108	14.68	0.66	4.47	0.00	0.00	0.00	0.00	0.41	2.78	0.30	2.02	0.83	5.64
<i>C. albicans</i> Mod Pos <sup>1</sup>	107	14.37	0.66	4.58	0.14	0.99	0.00	0.00	0.35	2.42	0.28	1.98	0.81	5.64
<i>C. glabrata</i> Low Pos	106	21.36	0.84	3.94	0.18	0.84	0.00	0.00	0.68	3.17	0.62	2.89	1.26	5.88
<i>C. glabrata</i> Mod Pos	107	20.54	0.99	4.83	0.30	1.46	0.00	0.00	0.76	3.70	0.48	2.34	1.37	6.68
<i>T. vaginalis</i> Low Pos	108	24.32	1.16	4.77	0.00	0.00	0.00	0.00	0.90	3.71	0.60	2.48	1.59	6.54
<i>T. vaginalis</i> Mod Pos	107	23.09	1.18	5.13	0.00	0.00	0.00	0.00	0.86	3.71	0.56	2.41	1.56	6.77

CV = coefficient of variation, Mod = moderate, Pos = positive, SD = standard deviation

<sup>1</sup> C<sub>95</sub> (*C. albicans* panels) is defined relative to clinical cutoff.

Note: In the event that variability from some factors is numerically negative, SD and CV are shown as 0.00.

## Panther System Clinical Performance

### Performance Characteristics in Symptomatic Subjects

A prospective, multi-center clinical study was conducted to establish the clinical performance characteristics of the Aptima CV/TV assay on the Panther system. Female subjects presenting with symptoms of vaginitis were enrolled at 21 geographically and ethnically diverse US clinical sites, including private and academic family practice, obstetric-gynecologic, family planning, public health, sexually transmitted infections (STI), and medical group clinics, and clinical research centers.

Five (5) vaginal swab samples were collected from each subject: one clinician-collected swab sample and one patient-collected swab sample were collected using the Aptima Multitest Swab Specimen Collection Kit for Aptima CV/TV assay testing, and three additional vaginal swab samples were collected for reference testing. The following reference methods were used for all subjects:

- *Candida* species group (C spp) and *C. glabrata* infection statuses were determined separately using Sabouraud dextrose and chromogenic culture of a clinician-collected swab sample, followed by PCR/bi-directional sequencing. For subjects with positive culture results (i.e., growth of any *Candida* on either culture plate), both Aptima swab samples leftover after testing with the Aptima CV/TV assay were used for PCR/bi-directional sequencing to determine whether C spp or *C. glabrata* were present. A positive sequencing result for C spp in either Aptima swab sample type was sufficient to establish a reference result positive for C spp in both Aptima swab types, and either a negative *Candida* culture result or a negative PCR/bi-directional sequencing result for both Aptima swab samples was sufficient to establish a reference result negative for C spp in both Aptima swab types; a similar algorithm was followed for establishing *C. glabrata* reference results.
- *T. vaginalis* patient infection status (PIS) was determined using a composite result from two FDA-cleared assays for *T. vaginalis*, one molecular assay and one culture-based assay. A positive result for at least one assay was sufficient to establish a reference result positive for *T. vaginalis* for both Aptima swab types, and a negative result for both assays was sufficient to establish a reference result negative for *T. vaginalis* for both Aptima swab types.

Aptima samples were tested with the Aptima CV/TV assay on the Panther system at three sites.

Performance characteristics for each prospectively-collected sample type, with corresponding 2-sided 95% Score confidence intervals (CIs), were estimated relative to *Candida* species group and *C. glabrata* infection status and *T. vaginalis* PIS.

Of the 1519 symptomatic subjects enrolled, 17 subjects were withdrawn, and six subjects were not evaluable due to final invalid Aptima CV/TV assay results (n = 1), missing vaginal swabs (n = 1), or unknown *Candida* infection status or *T. vaginalis* PIS (n = 4). The remaining 1496 subjects were evaluable for at least one analyte in at least one of the sample types. Table 4 shows the demographics of evaluable subjects.

Table 4: Demographics of Evaluable Subjects

Characteristics		Total
Total, N	N	1496
Age (years)	Mean ± SD	35.3 ± 11.76
	Median	33.0
	Range	14-79
Age category (years), n (%)	14-17	5 (0.3)
	18-29	554 (37.0)
	30-39	480 (32.1)
	40-49	247 (16.5)
	>50	210 (14.0)
Race/Ethnicity, n (%)	Asian	73 (4.9)
	Black or African American	752 (50.3)
	White (Hispanic or Latino)	268 (17.9)
	White (Not Hispanic or Latino)	339 (22.7)
	Other <sup>1</sup>	64 (4.3)

<sup>1</sup> Includes patient-reported other, mixed, and unknown races.

For the 1496 evaluable subjects, 1485 clinician-collected vaginal swab samples and 1477 patient-collected vaginal swab samples were included in the analyses for *Candida* species group, 1483 clinician-collected vaginal swab samples and 1475 patient-collected vaginal swab samples were included in the analyses for *C. glabrata*, and 1438 clinician-collected vaginal swab samples and 1433 patient-collected vaginal swab samples were included in the analyses for *T. vaginalis*.

### Candida Species Group Performance Characteristics

The sensitivity and specificity of the Aptima CV/TV assay for the detection of *Candida* species group are shown for both sample types overall and by site in Table 5. Assay performance is shown stratified by race/ethnicity in Table 6, and by clinical condition in Table 7.

Table 5: Candida Species Group Performance Characteristics by Collection Site in Symptomatic Women

Site	Clinician-collected Vaginal Swabs				Patient-collected Vaginal Swabs			
	N	Prev (%)	Sensitivity % (95% CI) <sup>1</sup>	Specificity % (95% CI) <sup>1</sup>	N	Prev (%)	Sensitivity % (95% CI) <sup>1</sup>	Specificity % (95% CI) <sup>1</sup>
<b>All</b>	<b>1485</b>	<b>28.6</b>	<b>91.7</b> <b>(88.7-94.0)</b> <b>389/424</b>	<b>94.9</b> <b>(93.4-96.1)</b> <b>1007/1061</b>	<b>1477</b>	<b>28.6</b>	<b>92.9</b> <b>(90.0-95.0)</b> <b>392/422</b>	<b>91.0</b> <b>(89.1-92.6)</b> <b>960/1055</b>
1	20	25.0	60.0 (23.1-88.2) 3/5	100 (79.6-100) 15/15	20	25.0	60.0 (23.1-88.2) 3/5	93.3 (70.2-98.8) 14/15
2	5	0.0	NC	80.0 (37.6-96.4) 4/5	5	0.0	NC	100 (56.6-100) 5/5
3	22	54.5	91.7 (64.6-98.5) 11/12	90.0 (59.6-98.2) 9/10	22	54.5	91.7 (64.6-98.5) 11/12	90.0 (59.6-98.2) 9/10
4	216	22.2	85.4 (72.8-92.8) 41/48	94.6 (90.1-97.2) 159/168	213	22.5	85.4 (72.8-92.8) 41/48	88.5 (82.7-92.5) 146/165
5	147	24.5	88.9 (74.7-95.6) 32/36	94.6 (88.7-97.5) 105/111	144	24.3	91.4 (77.6-97.0) 32/35	91.7 (85.0-95.6) 100/109
6	72	31.9	100 (85.7-100) 23/23	98.0 (89.3-99.6) 48/49	72	31.9	95.7 (79.0-99.2) 22/23	95.9 (86.3-98.9) 47/49
7	197	21.8	93.0 (81.4-97.6) 40/43	94.8 (90.1-97.3) 146/154	197	21.8	90.7 (78.4-96.3) 39/43	89.6 (83.8-93.5) 138/154
8	1	0.0	NC	100 (20.7-100) 1/1	1	0.0	NC	100 (20.7-100) 1/1
9	108	43.5	87.2 (74.8-94.0) 41/47	100 (94.1-100) 61/61	108	43.5	93.6 (82.8-97.8) 44/47	90.2 (80.2-95.4) 55/61
10	17	35.3	100 (61.0-100) 6/6	81.8 (52.3-94.9) 9/11	17	35.3	100 (61.0-100) 6/6	72.7 (43.4-90.3) 8/11
11	71	26.8	89.5 (68.6-97.1) 17/19	96.2 (87.0-98.9) 50/52	72	26.4	94.7 (75.4-99.1) 18/19	96.2 (87.2-99.0) 51/53
12	138	31.9	95.5 (84.9-98.7) 42/44	95.7 (89.6-98.3) 90/94	135	31.1	95.2 (84.2-98.7) 40/42	93.5 (86.6-97.0) 87/93
13	69	27.5	100 (83.2-100) 19/19	96.0 (86.5-98.9) 48/50	69	29.0	95.0 (76.4-99.1) 19/20	93.9 (83.5-97.9) 46/49
14	9	44.4	100 (51.0-100) 4/4	100 (56.6-100) 5/5	9	44.4	100 (51.0-100) 4/4	100 (56.6-100) 5/5
15	4	50.0	100 (34.2-100) 2/2	100 (34.2-100) 2/2	4	50.0	100 (34.2-100) 2/2	100 (34.2-100) 2/2
16	30	43.3	84.6 (57.8-95.7) 11/13	94.1 (73.0-99.0) 16/17	30	43.3	92.3 (66.7-98.6) 12/13	88.2 (65.7-96.7) 15/17

Table 5: *Candida Species Group Performance Characteristics by Collection Site in Symptomatic Women*

Clinician-collected Vaginal Swabs					Patient-collected Vaginal Swabs			
Site	N	Prev (%)	Sensitivity % (95% CI) <sup>1</sup>	Specificity % (95% CI) <sup>1</sup>	N	Prev (%)	Sensitivity % (95% CI) <sup>1</sup>	Specificity % (95% CI) <sup>1</sup>
17	80	35.0	92.9 (77.4-98.0) 26/28	92.3 (81.8-97.0) 48/52	80	35.0	96.4 (82.3-99.4) 27/28	90.4 (79.4-95.8) 47/52
18	86	30.2	92.3 (75.9-97.9) 24/26	88.3 (77.8-94.2) 53/60	86	30.2	96.2 (81.1-99.3) 25/26	88.3 (77.8-94.2) 53/60
19	75	41.3	100 (89.0-100) 31/31	95.5 (84.9-98.7) 42/44	75	41.3	100 (89.0-100) 31/31	88.6 (76.0-95.0) 39/44
20	39	7.7	100 (43.9-100) 3/3	97.2 (85.8-99.5) 35/36	39	7.7	100 (43.9-100) 3/3	97.2 (85.8-99.5) 35/36
21	79	19.0	86.7 (62.1-96.3) 13/15	95.3 (87.1-98.4) 61/64	79	19.0	86.7 (62.1-96.3) 13/15	89.1 (79.1-94.6) 57/64

CI = confidence interval, NC = not calculable, Prev = prevalence

<sup>1</sup> Score CI.



Table 6: *Candida* Species Group Performance Characteristics by Race/Ethnicity in Symptomatic Women

Specimen Type	Race/Ethnicity	N	Prev (%)	Sensitivity % (95% CI) <sup>1</sup>	Specificity % (95% CI) <sup>1</sup>
Clinician-collected Vaginal Swabs	All	1485	28.6	91.7 (88.7-94.0) 389/424	94.9 (93.4-96.1) 1007/1061
	Asian	73	26.0	100 (83.2-100) 19/19	94.4 (84.9-98.1) 51/54
	Black/African-American	747	30.4	90.7 (86.3-93.9) 206/227	94.0 (91.7-95.8) 489/520
	White (Hispanic/Latino)	265	28.7	93.4 (85.5-97.2) 71/76	93.7 (89.2-96.3) 177/189
	White (Not Hispanic/Latino)	336	23.8	91.3 (83.0-95.7) 73/80	97.7 (95.0-98.9) 250/256
	Other <sup>2</sup>	64	34.4	90.9 (72.2-97.5) 20/22	95.2 (84.2-98.7) 40/42
Patient-collected Vaginal Swabs	All	1477	28.6	92.9 (90.0-95.0) 392/422	91.0 (89.1-92.6) 960/1055
	Asian	71	25.4	100 (82.4-100) 18/18	90.6 (79.7-95.9) 48/53
	Black/African-American	745	30.6	90.8 (86.3-93.9) 207/228	89.4 (86.4-91.7) 462/517
	White (Hispanic/Latino)	265	28.7	93.4 (85.5-97.2) 71/76	89.9 (84.8-93.5) 170/189
	White (Not Hispanic/Latino)	332	23.5	96.2 (89.3-98.7) 75/78	95.3 (91.9-97.3) 242/254
	Other <sup>2</sup>	64	34.4	95.5 (78.2-99.2) 21/22	90.5 (77.9-96.2) 38/42

CI = confidence interval, Prev = prevalence

<sup>1</sup> Score CI.<sup>2</sup> Includes patient-reported other, mixed, and unknown races.

Table 7: *Candida Species Group Performance Characteristics by Clinical Condition in Symptomatic Women*

Collection Type	Clinical Condition	N <sup>1</sup>	Prev (%)	Sensitivity % (95% CI) <sup>2</sup>	Specificity % (95% CI) <sup>2</sup>
Clinician-collected Vaginal Swabs	<b>All</b>	<b>1485</b>	<b>28.6</b>	<b>91.7 (88.7-94.0)</b> <b>389/424</b>	<b>94.9 (93.4-96.1)</b> <b>1007/1061</b>
	Use of antibiotics	5	60.0	66.7 (20.8-93.9) 2/3	50.0 (9.5-90.5) 1/2
	Use of antifungals	8	37.5	100 (43.9-100) 3/3	100 (56.6-100) 5/5
	Use of estrogen therapy	2	0.0	NC	100 (34.2-100) 2/2
	Recurrent symptoms of vaginitis in the last 12 months	863	28.6	89.9 (85.5-93.0) 222/247	95.0 (92.9-96.4) 585/616
	Unprotected intercourse in the last 24 hours	96	27.1	84.6 (66.5-93.8) 22/26	92.9 (84.3-96.9) 65/70
	Pregnant	20	55.0	100 (74.1-100) 11/11	100 (70.1-100) 9/9
	With menses	118	30.5	94.4 (81.9-98.5) 34/36	97.6 (91.5-99.3) 80/82
	Without menses	1210	29.6	92.5 (89.2-94.8) 331/358	94.4 (92.6-95.7) 804/852
	Post-menopausal	157	19.1	80.0 (62.7-90.5) 24/30	96.9 (92.2-98.8) 123/127
Patient-collected Vaginal Swabs	<b>All</b>	<b>1477</b>	<b>28.6</b>	<b>92.9 (90.0-95.0)</b> <b>392/422</b>	<b>91.0 (89.1-92.6)</b> <b>960/1055</b>
	Use of antibiotics	5	60.0	66.7 (20.8-93.9) 2/3	0.0 (0.0-65.8) 0/2
	Use of antifungals	8	37.5	100 (43.9-100) 3/3	100 (56.6-100) 5/5
	Use of estrogen therapy	2	0.0	NC	100 (34.2-100) 2/2
	Recurrent symptoms of vaginitis in the last 12 months	859	28.6	90.7 (86.4-93.7) 223/246	91.2 (88.7-93.2) 559/613
	Unprotected intercourse in the last 24 hours	95	27.4	88.5 (71.0-96.0) 23/26	85.5 (75.3-91.9) 59/69
	Pregnant	21	52.4	100 (74.1-100) 11/11	100 (72.2-100) 10/10
	With menses	116	30.2	97.1 (85.5-99.5) 34/35	88.9 (80.2-94.0) 72/81
	Without menses	1207	29.7	93.0 (89.9-95.2) 333/358	91.0 (88.9-92.8) 773/849
	Post-menopausal	154	18.8	86.2 (69.4-94.5) 25/29	92.0 (85.9-95.6) 115/125

CI = confidence interval, NC = not calculable, Prev = prevalence

<sup>1</sup> Subjects may report multiple clinical conditions; sum of subject numbers in all subgroups does not equal the total number of subjects.

<sup>2</sup> Score CI.

## Candida glabrata Performance Characteristics

The sensitivity and specificity of the Aptima CV/TV assay for the detection of *Candida glabrata* are shown for both sample types overall and by site in Table 8. Assay performance is shown stratified by race/ethnicity in Table 9, and by clinical condition in Table 10.

Table 8: *Candida glabrata* Performance Characteristics by Collection Site in Symptomatic Women

Site	Clinician-collected Vaginal Swabs				Patient-collected Vaginal Swabs			
	N	Prev (%)	Sensitivity % (95% CI) <sup>1</sup>	Specificity % (95% CI) <sup>1</sup>	N	Prev (%)	Sensitivity % (95% CI) <sup>1</sup>	Specificity % (95% CI) <sup>1</sup>
<b>All</b>	<b>1483</b>	<b>4.0</b>	<b>84.7</b> <b>(73.5-91.8)</b> <b>50/59<sup>2</sup></b>	<b>99.1</b> <b>(98.4-99.5)</b> <b>1411/1424<sup>3</sup></b>	<b>1475</b>	<b>3.9</b>	<b>86.2</b> <b>(75.1-92.8)</b> <b>50/58<sup>4</sup></b>	<b>98.7</b> <b>(98.0-99.2)</b> <b>1399/1417<sup>5</sup></b>
1	20	5.0	100 (20.7-100) 1/1	100 (83.2-100) 19/19	20	5.0	100 (20.7-100) 1/1	100 (83.2-100) 19/19
2	5	0.0	NC	100 (56.6-100) 5/5	5	0.0	NC	100 (56.6-100) 5/5
3	22	0.0	NC	100 (85.1-100) 22/22	22	0.0	NC	100 (85.1-100) 22/22
4	215	5.6	66.7 (39.1-86.2) 8/12	98.5 (95.8-99.5) 200/203	213	5.6	75.0 (46.8-91.1) 9/12	97.0 (93.6-98.6) 195/201
5	147	4.8	100 (64.6-100) 7/7	100 (97.3-100) 140/140	144	4.9	100 (64.6-100) 7/7	99.3 (96.0-99.9) 136/137
6	72	2.8	100 (34.2-100) 2/2	98.6 (92.3-99.7) 69/70	72	2.8	100 (34.2-100) 2/2	98.6 (92.3-99.7) 69/70
7	197	7.1	71.4 (45.4-88.3) 10/14	97.3 (93.8-98.8) 178/183	197	7.1	71.4 (45.4-88.3) 10/14	97.8 (94.5-99.1) 179/183
8	1	0.0	NC	100 (20.7-100) 1/1	1	0.0	NC	100 (20.7-100) 1/1
9	108	1.9	100 (34.2-100) 2/2	100 (96.5-100) 106/106	108	1.9	100 (34.2-100) 2/2	99.1 (94.8-99.8) 105/106
10	17	5.9	100 (20.7-100) 1/1	100 (80.6-100) 16/16	17	5.9	100 (20.7-100) 1/1	100 (80.6-100) 16/16
11	71	4.2	100 (43.9-100) 3/3	98.5 (92.1-99.7) 67/68	72	4.2	100 (43.9-100) 3/3	98.6 (92.2-99.7) 68/69
12	138	2.9	100 (51.0-100) 4/4	100 (97.2-100) 134/134	135	2.2	100 (43.9-100) 3/3	99.2 (95.8-99.9) 131/132
13	69	1.4	100 (20.7-100) 1/1	100 (94.7-100) 68/68	68	1.5	100 (20.7-100) 1/1	98.5 (92.0-99.7) 66/67
14	9	0.0	NC	100 (70.1-100) 9/9	9	0.0	NC	100 (70.1-100) 9/9

Table 8: *Candida glabrata* Performance Characteristics by Collection Site in Symptomatic Women

Site	Clinician-collected Vaginal Swabs				Patient-collected Vaginal Swabs			
	N	Prev (%)	Sensitivity % (95% CI) <sup>1</sup>	Specificity % (95% CI) <sup>1</sup>	N	Prev (%)	Sensitivity % (95% CI) <sup>1</sup>	Specificity % (95% CI) <sup>1</sup>
15	4	0.0	NC	100 (51.0-100) 4/4	4	0.0	NC	100 (51.0-100) 4/4
16	30	0.0	NC	96.7 (83.3-99.4) 29/30	30	0.0	NC	96.7 (83.3-99.4) 29/30
17	80	2.5	50.0 (9.5-90.5) 1/2	98.7 (93.1-99.8) 77/78	80	2.5	50.0 (9.5-90.5) 1/2	100 (95.3-100) 78/78
18	85	1.2	100 (20.7-100) 1/1	100 (95.6-100) 84/84	85	1.2	100 (20.7-100) 1/1	100 (95.6-100) 84/84
19	75	5.3	100 (51.0-100) 4/4	100 (94.9-100) 71/71	75	5.3	100 (51.0-100) 4/4	100 (94.9-100) 71/71
20	39	5.1	100 (34.2-100) 2/2	100 (90.6-100) 37/37	39	5.1	100 (34.2-100) 2/2	100 (90.6-100) 37/37
21	79	3.8	100 (43.9-100) 3/3	98.7 (92.9-99.8) 75/76	79	3.8	100 (43.9-100) 3/3	98.7 (92.9-99.8) 75/76

CI = confidence interval, NC = not calculable, Prev = prevalence

<sup>1</sup> Score CI.

<sup>2</sup> All 9 samples with false negative results showed no growth of *C. glabrata* on chromogenic agar.

<sup>3</sup> Of the 13 samples with false positive results, 2 showed high (4+) growth, 2 showed low ( $\leq 2+$ ) growth, and 9 showed no growth of *C. glabrata* on chromogenic agar.

<sup>4</sup> Of the 8 samples with false negative results, 7 showed no growth and 1 showed high (4+) growth of *C. glabrata* on chromogenic agar.

<sup>5</sup> Of the 18 samples with false positive results, 2 showed high (4+) growth, 2 showed low ( $\leq 2+$ ) growth, and 14 showed no growth of *C. glabrata* on chromogenic agar.

Table 9: *Candida glabrata* Performance Characteristics by Race/Ethnicity in Symptomatic Women

Specimen Type	Race/Ethnicity	N	Prev (%)	Sensitivity % (95% CI) <sup>1</sup>	Specificity % (95% CI) <sup>1</sup>
Clinician-collected Vaginal Swabs	All	1483	4.0	84.7 (73.5-91.8) 50/59	99.1 (98.4-99.5) 1411/1424
	Asian	72	4.2	100 (43.9-100) 3/3	100 (94.7-100) 69/69
	Black/African-American	747	4.1	74.2 (56.8-86.3) 23/31	98.7 (97.6-99.3) 707/716
	White (Hispanic/Latino)	264	3.0	87.5 (52.9-97.8) 7/8	99.6 (97.8-99.9) 255/256
	White (Not Hispanic/Latino)	336	4.2	100 (78.5-100) 14/14	99.1 (97.3-99.7) 319/322
	Other <sup>2</sup>	64	4.7	100 (43.9-100) 3/3	100 (94.1-100) 61/61
Patient-collected Vaginal Swabs	All	1475	3.9	86.2 (75.1-92.8) 50/58	98.7 (98.0-99.2) 1399/1417
	Asian	71	4.2	100 (43.9-100) 3/3	98.5 (92.1-99.7) 67/68
	Black/African-American	744	4.2	77.4 (60.2-88.6) 24/31	98.7 (97.6-99.3) 704/713
	White (Hispanic/Latino)	264	3.0	87.5 (52.9-97.8) 7/8	99.2 (97.2-99.8) 254/256
	White (Not Hispanic/Latino)	332	3.9	100 (77.2-100) 13/13	98.4 (96.4-99.3) 314/319
	Other <sup>2</sup>	64	4.7	100 (43.9-100) 3/3	98.4 (91.3-99.7) 60/61

CI = confidence interval, Prev = prevalence

<sup>1</sup> Score CI.

<sup>2</sup> Includes patient-reported other, mixed, and unknown races.

Table 10: *Candida glabrata* Performance Characteristics by Clinical Condition in Symptomatic Women

Collection Type	Clinical Condition	N <sup>1</sup>	Prev (%)	Sensitivity % (95% CI) <sup>2</sup>	Specificity % (95% CI) <sup>2</sup>
Clinician-collected Vaginal Swabs	All	1483	4.0	84.7 (73.5-91.8) 50/59	99.1 (98.4-99.5) 1411/1424
	Use of antibiotics	5	20.0	100 (20.7-100) 1/1	100 (51.0-100) 4/4
	Use of antifungals	8	12.5	100 (20.7-100) 1/1	100 (64.6-100) 7/7
	Use of estrogen therapy	2	0.0	NC	100 (34.2-100) 2/2
	Recurrent symptoms of vaginitis in the last 12 months	861	3.9	88.2 (73.4-95.3) 30/34	99.0 (98.1-99.5) 819/827
	Unprotected intercourse in the last 24 hours	96	4.2	100 (51.0-100) 4/4	100 (96.0-100) 92/92
	Pregnant	20	0.0	NC	95.0 (76.4-99.1) 19/20
	With menses	117	2.6	100 (43.9-100) 3/3	100 (96.7-100) 114/114
	Without menses	1209	3.8	80.4 (66.8-89.3) 37/46	99.1 (98.4-99.5) 1153/1163
	Post-menopausal	157	6.4	100 (72.2-100) 10/10	98.0 (94.2-99.3) 144/147
Patient-collected Vaginal Swabs	All	1475	3.9	86.2 (75.1-92.8) 50/58	98.7 (98.0-99.2) 1399/1417
	Use of antibiotics	5	20.0	100 (20.7-100) 1/1	100 (51.0-100) 4/4
	Use of antifungals	8	12.5	100 (20.7-100) 1/1	100 (64.6-100) 7/7
	Use of estrogen therapy	2	0.0	NC	100 (34.2-100) 2/2
	Recurrent symptoms of vaginitis in the last 12 months	858	4.0	91.2 (77.0-97.0) 31/34	99.2 (98.3-99.6) 817/824
	Unprotected intercourse in the last 24 hours	95	4.2	100 (51.0-100) 4/4	100 (95.9-100) 91/91
	Pregnant	21	0.0	NC	90.5 (71.1-97.3) 19/21
	With menses	116	2.6	100 (43.9-100) 3/3	100 (96.7-100) 113/113
	Without menses	1205	3.8	84.8 (71.8-92.4) 39/46	99.0 (98.2-99.4) 1147/1159
	Post-menopausal	154	5.8	88.9 (56.5-98.0) 8/9	95.9 (91.3-98.1) 139/145

CI = confidence interval, NC = not calculable, Prev = prevalence

<sup>1</sup> Subjects may report multiple clinical conditions; sum of subject numbers in all subgroups does not equal the total number of subjects.

<sup>2</sup> Score CI.

Due to anticipated low prevalence of *Candida glabrata*, the performance of the Aptima CV/TV assay was also assessed using contrived specimens to supplement the data collected in the clinical study. Contrived specimens were prepared by spiking five different strains of *Candida glabrata* in simulated vaginal swab matrix, at concentrations of 3X, 10X, and 20X the assay's

LoD. True negative specimens containing matrix only were also tested. Agreement was 100% across all contrived specimens (see Table 11).

Table 11: *Candida glabrata* Contrived Specimen Agreement

	N	Aptima <i>C. glabrata</i> Positive	Aptima <i>C. glabrata</i> Negative	PPA % (95% CI) <sup>1</sup>	NPA % (95% CI) <sup>1</sup>
True Negative	60	0	60	NC	100 (94.0-100)
Low Positive (3X LoD)	30	30	0	100 (88.6-100)	NC
Moderate Positive  10X LoD	15	15	0	100 (79.6-100)	NC
High Positive (20X LoD)	15	15	0	100 (79.6-100)	NC

NC = not calculable, LoD = limit of detection, NPA = negative percent agreement, PPA = positive percent agreement

<sup>1</sup> Score CI.

## Trichomonas vaginalis Performance Characteristics

The sensitivity and specificity of the Aptima CV/TV assay for the detection of *Trichomonas vaginalis* are shown for both sample types overall and by site in Table 12. Assay performance is shown stratified by race/ethnicity in Table 13, and by clinical condition in Table 14.

Table 12: *Trichomonas vaginalis* Performance Characteristics by Collection Site in Symptomatic Women

Site	Clinician-collected Vaginal Swabs				Patient-collected Vaginal Swabs			
	N	Prev (%)	Sensitivity % (95% CI) <sup>1</sup>	Specificity % (95% CI) <sup>1</sup>	N	Prev (%)	Sensitivity % (95% CI) <sup>1</sup>	Specificity % (95% CI) <sup>1</sup>
All	1438	9.9	96.5 (92.0-98.5) 137/142 <sup>2</sup>	95.1 (93.8-96.2) 1233/1296 <sup>3</sup>	1433	9.8	97.1 (92.9-98.9) 136/140 <sup>4</sup>	98.9 (98.2-99.4) 1279/1293 <sup>5</sup>
1	16	6.3	100 (20.7-100) 1/1	100 (79.6-100) 15/15	16	6.3	100 (20.7-100) 1/1	100 (79.6-100) 15/15
2	1	0.0	NC	100 (20.7-100) 1/1	1	0.0	NC	100 (20.7-100) 1/1
3	21	9.5	100 (34.2-100) 2/2	100 (83.2-100) 19/19	21	9.5	100 (34.2-100) 2/2	100 (83.2-100) 19/19
4	213	17.4	97.3 (86.2-99.5) 36/37	83.5 (77.3-88.3) 147/176	211	17.1	100 (90.4-100) 36/36	98.9 (95.9-99.7) 173/175
5	145	7.6	100 (74.1-100) 11/11	98.5 (94.7-99.6) 132/134	143	7.7	100 (74.1-100) 11/11	100 (97.2-100) 132/132
6	68	1.5	100 (20.7-100) 1/1	98.5 (92.0-99.7) 66/67	68	1.5	100 (20.7-100) 1/1	100 (94.6-100) 67/67

Table 12: *Trichomonas vaginalis* Performance Characteristics by Collection Site in Symptomatic Women

Clinician-collected Vaginal Swabs					Patient-collected Vaginal Swabs			
Site	N	Prev (%)	Sensitivity % (95% CI) <sup>1</sup>	Specificity % (95% CI) <sup>1</sup>	N	Prev (%)	Sensitivity % (95% CI) <sup>1</sup>	Specificity % (95% CI) <sup>1</sup>
7	197	23.9	100 (92.4-100) 47/47	83.3 (76.6-88.4) 125/150	197	23.9	100 (92.4-100) 47/47	93.3 (88.2-96.3) 140/150
8	1	100.0	100 (20.7-100) 1/1	NC	1	100.0	100 (20.7-100) 1/1	NC
9	105	3.8	100 (51.0-100) 4/4	100 (96.3-100) 101/101	105	3.8	100 (51.0-100) 4/4	100 (96.3-100) 101/101
10	17	0.0	NC	100 (81.6-100) 17/17	17	0.0	NC	100 (81.6-100) 17/17
11	70	7.1	80.0 (37.6-96.4) 4/5	93.8 (85.2-97.6) 61/65	71	7.0	80.0 (37.6-96.4) 4/5	100 (94.5-100) 66/66
12	130	3.1	75.0 (30.1-95.4) 3/4	100 (97.0-100) 126/126	129	3.1	75.0 (30.1-95.4) 3/4	100 (97.0-100) 125/125
13	69	10.1	100 (64.6-100) 7/7	96.8 (89.0-99.1) 60/62	69	10.1	100 (64.6-100) 7/7	98.4 (91.4-99.7) 61/62
14	8	0.0	NC	100 (67.6-100) 8/8	8	0.0	NC	100 (67.6-100) 8/8
15	4	25.0	0.0 (0.0-79.3) 0/1	100 (43.9-100) 3/3	4	25.0	0.0 (0.0-79.3) 0/1	100 (43.9-100) 3/3
16	28	10.7	100 (43.9-100) 3/3	100 (86.7-100) 25/25	28	10.7	100 (43.9-100) 3/3	100 (86.7-100) 25/25
17	74	2.7	100 (34.2-100) 2/2	100 (94.9-100) 72/72	74	2.7	100 (34.2-100) 2/2	98.6 (92.5-99.8) 71/72
18	83	4.8	100 (51.0-100) 4/4	100 (95.4-100) 79/79	83	4.8	100 (51.0-100) 4/4	100 (95.4-100) 79/79
19	71	4.2	66.7 (20.8-93.9) 2/3	100 (94.7-100) 68/68	71	4.2	66.7 (20.8-93.9) 2/3	100 (94.7-100) 68/68
20	39	0.0	NC	100 (91.0-100) 39/39	39	0.0	NC	100 (91.0-100) 39/39
21	78	11.5	100 (70.1-100) 9/9	100 (94.7-100) 69/69	77	10.4	100 (67.6-100) 8/8	100 (94.7-100) 69/69

CI = confidence interval, NC = not calculable, Prev = prevalence

<sup>1</sup> Score CI.

<sup>2</sup> Of the 5 samples with false negative results, 3 were negative with a second FDA-cleared TV NAAT.

<sup>3</sup> Of the 63 samples with false positive results, 56 were positive with a second FDA-cleared TV NAAT.

<sup>4</sup> Of the 4 samples with false negative results, 3 were negative with a second FDA-cleared TV NAAT.

<sup>5</sup> Of the 14 samples with false positive results, 8 were positive with a second FDA-cleared TV NAAT.



Table 13: *Trichomonas vaginalis* Performance Characteristics by Race/Ethnicity in Symptomatic Women

Specimen Type	Race/Ethnicity	N	Prev (%)	Sensitivity % (95% CI) <sup>1</sup>	Specificity % (95% CI) <sup>1</sup>
Clinician-collected Vaginal Swabs	All	1438	9.9	96.5 (92.0-98.5) 137/142	95.1 (93.8-96.2) 1233/1296
	Asian	67	6.0	100 (51.0-100) 4/4	98.4 (91.5-99.7) 62/63
	Black/African-American	727	14.2	98.1 (93.2-99.5) 101/103	93.3 (91.0-95.0) 582/624
	White (Hispanic/Latino)	257	6.6	94.1 (73.0-99.0) 16/17	95.0 (91.5-97.1) 228/240
	White (Not Hispanic/Latino)	326	4.0	84.6 (57.8-95.7) 11/13	97.4 (95.0-98.7) 305/313
	Other <sup>2</sup>	61	8.2	100 (56.6-100) 5/5	100 (93.6-100) 56/56
Patient-collected Vaginal Swabs	All	1433	9.8	97.1 (92.9-98.9) 136/140	98.9 (98.2-99.4) 1279/1293
	Asian	66	6.1	100 (51.0-100) 4/4	100 (94.2-100) 62/62
	Black/African-American	724	14.0	98.0 (93.1-99.5) 99/101	98.7 (97.5-99.3) 615/623
	White (Hispanic/Latino)	258	6.6	94.1 (73.0-99.0) 16/17	97.9 (95.2-99.1) 236/241
	White (Not Hispanic/Latino)	324	4.0	92.3 (66.7-98.6) 12/13	99.7 (98.2-99.9) 310/311
	Other <sup>2</sup>	61	8.2	100 (56.6-100) 5/5	100 (93.6-100) 56/56

CI = confidence interval, Prev = prevalence

<sup>1</sup> Score CI.<sup>2</sup> Includes patient-reported other, mixed, and unknown races.

Table 14: *Trichomonas vaginalis* Performance Characteristics by Clinical Condition in Symptomatic Women

Collection Type	Clinical Condition	N <sup>1</sup>	Prev (%)	Sensitivity % (95% CI) <sup>2</sup>	Specificity % (95% CI) <sup>2</sup>
Clinician-collected Vaginal Swabs	<b>All</b>	<b>1438</b>	<b>9.9</b>	<b>96.5 (92.0-98.5)</b> <b>137/142</b>	<b>95.1 (93.8-96.2)</b> <b>1233/1296</b>
	Use of antibiotics	5	0.0	NC	100 (56.6-100) 5/5
	Use of antifungals	7	0.0	NC	100 (64.6-100) 7/7
	Use of estrogen therapy	2	0.0	NC	100 (34.2-100) 2/2
	Recurrent symptoms of vaginitis in the last 12 months	841	8.1	95.6 (87.8-98.5) 65/68	94.7 (92.9-96.1) 732/773
	Unprotected intercourse in the last 24 hours	94	12.8	91.7 (64.6-98.5) 11/12	96.3 (89.8-98.7) 79/82
	Pregnant	20	15.0	66.7 (20.8-93.9) 2/3	100 (81.6-100) 17/17
	With menses	112	9.8	90.9 (62.3-98.4) 10/11	97.0 (91.6-99.0) 98/101
	Without menses	1176	9.9	97.4 (92.7-99.1) 114/117	95.3 (93.8-96.4) 1009/1059
	Post-menopausal	150	9.3	92.9 (68.5-98.7) 13/14	92.6 (87.0-96.0) 126/136
Patient-collected Vaginal Swabs	<b>All</b>	<b>1433</b>	<b>9.8</b>	<b>97.1 (92.9-98.9)</b> <b>136/140</b>	<b>98.9 (98.2-99.4)</b> <b>1279/1293</b>
	Use of antibiotics	5	0.0	NC	100 (56.6-100) 5/5
	Use of antifungals	7	0.0	NC	100 (64.6-100) 7/7
	Use of estrogen therapy	2	0.0	NC	100 (34.2-100) 2/2
	Recurrent symptoms of vaginitis in the last 12 months	839	8.0	97.0 (89.8-99.2) 65/67	98.4 (97.3-99.1) 760/772
	Unprotected intercourse in the last 24 hours	93	12.9	100 (75.8-100) 12/12	100 (95.5-100) 81/81
	Pregnant	21	14.3	66.7 (20.8-93.9) 2/3	100 (82.4-100) 18/18
	With menses	112	9.8	90.9 (62.3-98.4) 10/11	99.0 (94.6-99.8) 100/101
	Without menses	1173	9.8	97.4 (92.6-99.1) 112/115	98.9 (98.0-99.4) 1046/1058
	Post-menopausal	148	9.5	100 (78.5-100) 14/14	99.3 (95.9-99.9) 133/134

CI = confidence interval, NC = not calculable, Prev = prevalence

<sup>1</sup> Subjects may report multiple clinical conditions; sum of subject numbers in all subgroups does not equal the total number of subjects.

<sup>2</sup> Score CI.

Co-detection rates, calculated for specimens with valid and conclusive Aptima CV/TV assay and reference results for all targets are reported in Table 15.

Table 15: Aptima CV/TV Co-detection Rates in Symptomatic Women

Analytes Detected	Clinician-collected Vaginal Swabs	Patient-collected Vaginal Swabs
<i>Candida</i> species group and <i>C. glabrata</i>	1.4% (21/1487)	1.6% (23/1478)
<i>Candida</i> species group and <i>T. vaginalis</i>	2.7% (40/1487)	3.1% (46/1478)
<i>Candida</i> species group and <i>C. glabrata</i> , and <i>T. vaginalis</i>	0.3% (4/1487)	0.3 (5/1478)
<i>C. glabrata</i> and <i>T. vaginalis</i>	0.2% (3/1487)	0.1% (1/1478)
<b>Total</b>	<b>4.6% (68/1487)</b>	<b>5.1% (75/1478)</b>

## Positivity Rates in Asymptomatic Women

The detection of an imbalance in the vaginal microbiome is relevant for treatment decisions. Although the Aptima CV/TV assay is not intended for use in testing samples from asymptomatic women, organisms associated with vulvovaginal candidiasis and detected by the Aptima CV/TV assay may also be present in asymptomatic women. Presence of the Aptima CV/TV assay targets was assessed in clinician-collected vaginal swab samples from 171 asymptomatic women. A summary of the detection rates for *Candida* species group and *Candida glabrata* as determined by the Aptima CV/TV assay, is shown in Table 16 for the multi-center study overall and by race/ethnicity.

Table 16: Positivity as Determined by the Aptima CV/TV Assay in Asymptomatic Women

	% Positivity (# positive/# tested with valid results)	
	<i>Candida</i> species group	<i>Candida glabrata</i>
<b>All</b>	<b>21.1% (36/171)</b>	<b>8.8% (15/171)</b>
<b>Asian</b>	0.0% (0/5)	0.0% (0/5)
<b>Black/African American</b>	28.0% (21/75)	12.0% (9/75)
<b>White (Hispanic/Latino)</b>	17.1% (7/41)	4.9% (2/41)
<b>White (Not Hispanic/Latino)</b>	11.6% (5/43)	7.0% (3/43)
<b>Other<sup>1</sup></b>	42.9% (3/7)	14.3% (1/7)

<sup>1</sup> Includes patient-reported other, mixed, and unknown races.

## Invalid Rates

A total of 3295 clinician- and patient-collected samples from symptomatic and asymptomatic subjects were processed in valid Aptima CV/TV runs to establish clinical performance. Of these, 1.7% had initial invalid results. Upon retest, 0.5% remained invalid and were excluded from all analyses.

## Panther System Analytical Performance

### Analytical Sensitivity

The analytical sensitivity/LoD of the Aptima CV/TV assay was determined by testing a series of panels consisting of target organisms diluted in pooled negative clinical specimens or simulated vaginal swab matrix (SVSM). A minimum of 20 replicates of each panel member were tested with each of the two reagent lots, for a minimum of 40 replicates per panel member. Probit analysis was performed to generate the 95% predicted detection limit for each organism. The predicted detection limits are shown in Table 17.

Table 17: Limit of Detection of the Aptima CV/TV Assay

Organism	Predicted Detection Limit	Concentration	Units
<i>C. albicans</i>	95%	4439	CFU/mL
<i>C. glabrata</i>	95%	41	CFU/mL
<i>C. parapsilosis</i> <sup>1</sup>	95%	9416	CFU/mL
<i>C. tropicalis</i> <sup>1</sup>	95%	811	CFU/mL
<i>C. dubliniensis</i> <sup>1</sup>	95%	1176	CFU/mL
<i>T. vaginalis</i>	95%	0.0024	Cells/mL

<sup>1</sup>Tested in simulated vaginal swab matrix

### Analytical Inclusivity

Five strains of each *Candida* target organism were tested using lysate targeting 3X LoD for *C. albicans*, *C. parapsilosis*, *C. tropicalis*, *C. dubliniensis* and *C. glabrata* in SVSM. Nine strains of *T. vaginalis* including a metronidazole resistant strain were tested with cell lysate targeting 3X LoD in SVSM. The Aptima CV/TV assay was positive for all *Candida* strains tested at 3X LoD. Eight of the nine *T. vaginalis* strains, including the metronidazole resistant strain, were detected at 3X LoD. One strain of *T. vaginalis* was detected at 4X LoD.

## Cross-Reactivity and Microbial Interference

Cross-reactivity and microbial interference with the Aptima CV/TV assay were evaluated in the presence of closely related and non-targeted organisms. A panel consisting of 64 organisms and human cell lines (Table 18) was tested in SVSM in the absence or presence of 3X LoD *C. albicans*, *C. glabrata* or *T. vaginalis*. No cross-reactivity or microbial interference was observed for any of the 64 organisms tested in the Aptima CV/TV assay at the concentrations listed in Table 18.

Table 18: Cross-Reactivity and Microbial Interference Panel

Microorganism	Concentration	Microorganism	Concentration
<i>Acinetobacter lwoffii</i>	1x10 <sup>6</sup> CFU/mL	Herpes simplex virus I	1x10 <sup>4</sup> TCID 50/mL
<i>Actinomyces israelii</i>	1x10 <sup>6</sup> CFU/mL	Herpes simplex virus II	1x10 <sup>4</sup> TCID 50/mL
<i>Alcaligenes faecalis</i>	1x10 <sup>6</sup> CFU/mL	<i>Klebsiella pneumoniae</i>	1x10 <sup>6</sup> CFU/mL
<i>Atopobium vaginae</i>	1x10 <sup>6</sup> CFU/mL	<i>Lactobacillus acidophilus</i>	1x10 <sup>6</sup> CFU/mL
<i>Bacteroides fragilis</i>	1x10 <sup>6</sup> CFU/mL	<i>Lactobacillus crispatus</i>	1x10 <sup>6</sup> CFU/mL
<i>Bifidobacterium adolescentis</i>	1x10 <sup>6</sup> CFU/mL	<i>Lactobacillus gasseri</i>	1x10 <sup>6</sup> CFU/mL
BVAB-1 <sup>1</sup>	1x10 <sup>6</sup> copies/mL	<i>Lactobacillus iners</i>	1x10 <sup>6</sup> CFU/mL
BVAB-2 <sup>1</sup>	1x10 <sup>6</sup> copies/mL	<i>Lactobacillus jensenii</i>	1x10 <sup>6</sup> CFU/mL
<i>Campylobacter jejuni</i>	1x10 <sup>6</sup> CFU/mL	<i>Lactobacillus mucosae</i>	1x10 <sup>6</sup> CFU/mL
<i>Candida catenulata</i>	1x10 <sup>6</sup> CFU/mL	<i>Leptotrichia buccalis</i>	1x10 <sup>6</sup> CFU/mL
<i>Candida famata</i> <sup>2</sup>	5x10 <sup>5</sup> CFU/mL	<i>Listeria monocytogenes</i>	1x10 <sup>6</sup> CFU/mL
<i>Candida guilliermondii</i>	1x10 <sup>6</sup> CFU/mL	<i>Megasphaera Type 1</i> <sup>1</sup>	1x10 <sup>6</sup> copies/mL
<i>Candida haemulonii</i>	1x10 <sup>6</sup> CFU/mL	<i>Mobiluncus curtisii</i>	1x10 <sup>6</sup> CFU/mL
<i>Candida inconspicua</i>	1x10 <sup>6</sup> CFU/mL	<i>Mycoplasma genitalium</i>	1x10 <sup>6</sup> CFU/mL
<i>Candida kefyr</i>	1x10 <sup>6</sup> CFU/mL	<i>Mycoplasma hominis</i>	1x10 <sup>6</sup> CFU/mL
<i>Candida krusei</i>	1x10 <sup>6</sup> CFU/mL	<i>Neisseria gonorrhoeae</i>	1x10 <sup>6</sup> CFU/mL
<i>Candida lusitanae</i>	1x10 <sup>6</sup> CFU/mL	<i>Peptostreptococcus magnus</i>	1x10 <sup>6</sup> CFU/mL
<i>Candida norvegica</i>	1x10 <sup>6</sup> CFU/mL	<i>Pentatrichomonas hominis</i>	1x10 <sup>5</sup> cells/mL
<i>Candida orthopsilosis</i>	1x10 <sup>6</sup> CFU/mL	<i>Pichia fermentans</i>	1x10 <sup>6</sup> CFU/mL
<i>Chlamydia trachomatis</i>	1x10 <sup>6</sup> IFU/mL	<i>Prevotella bivia</i>	1x10 <sup>6</sup> CFU/mL
<i>Clostridium difficile</i>	1x10 <sup>6</sup> CFU/mL	<i>Propionibacterium acnes</i>	1x10 <sup>6</sup> CFU/mL
<i>Corynebacterium genitalium</i>	1x10 <sup>6</sup> CFU/mL	<i>Proteus vulgaris</i>	1x10 <sup>6</sup> CFU/mL
<i>Cryptococcus neoformans</i>	1x10 <sup>6</sup> CFU/mL	SiHa cells	1x10 <sup>4</sup> cells/mL
<i>Eggerthella lenta</i>	1x10 <sup>6</sup> CFU/mL	<i>Sneathia amnii</i>	1x10 <sup>6</sup> CFU/mL
<i>Enterobacter cloacae</i>	1x10 <sup>6</sup> CFU/mL	<i>Staphylococcus aureus</i>	1x10 <sup>6</sup> CFU/mL
<i>Enterococcus faecalis</i>	1x10 <sup>6</sup> CFU/mL	<i>Staphylococcus epidermidis</i>	1x10 <sup>6</sup> CFU/mL
<i>Escherichia coli</i>	1x10 <sup>6</sup> CFU/mL	<i>Streptococcus agalactiae</i>	1x10 <sup>6</sup> CFU/mL
<i>Fusobacterium nucleatum</i>	1x10 <sup>6</sup> CFU/mL	<i>Streptococcus pyogenes</i>	1x10 <sup>6</sup> CFU/mL
<i>Gardnerella vaginalis</i>	1x10 <sup>6</sup> CFU/mL	<i>Treponema pallidum</i> <sup>1</sup>	1x10 <sup>6</sup> copies/mL
<i>Haemophilus ducreyi</i>	1x10 <sup>6</sup> CFU/mL	<i>Trichomonas tenax</i>	1x10 <sup>5</sup> cells/mL
HeLa cells	1x10 <sup>4</sup> Cells/mL	<i>Ureaplasma parvum</i>	1x10 <sup>6</sup> CFU/mL
HIV	1x10 <sup>5</sup> copies/mL	<i>Ureaplasma urealyticum</i>	1x10 <sup>6</sup> CFU/mL

CFU = Colony Forming Units; IFU = Inclusion Forming Units; TCID50 = Median Tissue Culture Infectious Dose

<sup>1</sup> In Vitro Transcript tested.

<sup>2</sup> Cross-reactivity with *Candida famata* was seen at concentrations higher than 5x10<sup>5</sup> CFU/mL.

## Interference

Potentially interfering substances were tested in the Aptima CV/TV assay. Panels were built in SVSM and evaluated for potential effects on assay sensitivity and specificity. Sensitivity performance was evaluated separately for *C. albicans*, *C. glabrata*, and *T. vaginalis* by spiking lysate at 3X LoD. Negative panels containing each substance were also evaluated for specificity.

No interference was observed in the presence of the following exogenous and endogenous substances tested at the concentrations listed in Table 19.

Table 19: Interfering Substances Panel

Substance	Final Concentration <sup>1</sup>
Whole Blood	5% V/V
Leukocytes	1x10 <sup>6</sup> cells/mL
Mucus	5% V/V
Seminal Fluid	5% V/V
Contraceptive Foam	5% W/V
Contraceptive Film	5% W/V
Tioconazole <sup>2</sup>	2% W/V
Douche	5% W/V
Progesterone	5% W/V
Estradiol	5% W/V
Acyclovir	5% W/V
Metronidazole	5% W/V
Hemorrhoidal Cream	5% W/V
Vaginal Moisturizing Gel <sup>3</sup>	0.5% W/V
Lubricant	5% V/V
Spermicide	5% W/V
Anti-fungal	5% W/V
Deodorant/Spray	5% W/V
Glacial Acetic Acid <sup>4</sup>	4% V/V
Vagisil Cream	5% W/V

W/V = weight by volume; V/V = volume by volume

<sup>1</sup> Final Concentration represents final concentration in the sample when tested on the Panther instrument.

<sup>2</sup> Tioconazole 6.5% Ointment: Interference was observed at  $\geq 3\%$  W/V for all analytes. No interference was observed at 2% W/V for all analytes.

<sup>3</sup> Vaginal Moisturizing Gel: Interference was observed at  $\geq 1\%$  W/V for *C. albicans*, 5% W/V for *C. glabrata*, and  $\geq 3\%$  W/V for *T. vaginalis*. No interference was observed at 0.5% W/V for *C. albicans*, 4% W/V for *C. glabrata*, and 2% W/V for *T. vaginalis*.

<sup>4</sup> Glacial Acetic Acid: Interference was observed at 5% V/V for *C. albicans*. No interference was observed at 4% V/V for *C. albicans*, 5% V/V for *C. glabrata*, and 5% V/V for *T. vaginalis*.

## Within Laboratory Precision

Within Lab Precision was evaluated on three Panther systems at one site. Three operators performed testing across 22 days and three reagent lots. Each operator performed two runs per day using a seven member panel. Each run consisted of three replicates of each panel member.

The panel members were made with *C. albicans*, *C. glabrata* or *T. vaginalis* in SVSM. The six positive panel members targeted *C. albicans* at Low and Moderate Positive, *C. glabrata* at Low and Moderate Positive, and *T. vaginalis* at Low and Moderate Positive. One Negative panel member contained matrix with no added target analytes.

The CV/TV percent positive results are presented in Table 20. Signal variability (TTime) of the Aptima CV/TV assay was also calculated for analyte positive panel members. Variability calculated between instruments, between operators, between lots, between days, between runs, within runs, and overall, is shown in Table 21.

Table 20: Precision - Agreement of Aptima CV/TV Assay with Expected Results

Panel (analyte composition)	Positive / Total n	Expected Positivity	Percent Positivity (95% CI)
Negative (SVSM)	0/162	0%	0 (0.0-2.3)
Low Positive ( <i>C. albicans</i> )	162/162	≥95%	100 (97.7-100.0)
Low Positive ( <i>C. glabrata</i> )	162/162	≥95%	100 (97.7-100.0)
Low Positive ( <i>T. vaginalis</i> )	162/162	≥95%	100 (97.7-100.0)
Moderate Positive ( <i>C. albicans</i> )	162/162	≥95%	100 (97.7-100.0)
Moderate Positive ( <i>C. glabrata</i> )	162/162	≥95%	100 (97.7-100.0)
Moderate Positive ( <i>T. vaginalis</i> )	162/162	≥95%	100 (97.7-100.0)

Table 21: Signal Variability of the Aptima CV/TV Assay by Panel Member

Panel Description	N	Mean TTime	Between Days		Between Instruments		Between Operators		Between Lots		Between Runs		Within Run		Total	
			SD	CV (%)	SD	CV (%)	SD	CV (%)	SD	CV (%)	SD	CV (%)	SD	CV (%)	SD	CV (%)
<i>C. albicans</i> Low Positive	162	14.96	0.12	0.82	0.00	0.00	0.24	1.59	0.54	3.58	0.23	1.52	0.28	1.84	0.70	4.66
<i>C. glabrata</i> Low Positive	162	21.07	0.00	0.00	0.15	0.69	0.25	1.18	0.14	0.65	0.19	0.89	0.40	1.91	0.55	2.59
<i>T. vaginalis</i> Low Positive	162	24.09	0.00	0.00	0.33	1.38	0.22	0.93	0.01	0.05	0.21	0.87	0.59	2.46	0.75	3.09
<i>C. albicans</i> Moderate Positive	162	14.62	0.11	0.72	0.00	0.00	0.22	1.47	0.43	2.95	0.26	1.77	0.24	1.62	0.60	4.14
<i>C. glabrata</i> Moderate Positive	162	20.63	0.00	0.00	0.00	0.00	0.26	1.27	0.31	1.50	0.26	1.25	0.52	2.51	0.71	3.42
<i>T. vaginalis</i> Moderate Positive	162	22.73	0.00	0.00	0.12	0.54	0.24	1.08	0.18	0.80	0.28	1.23	0.41	1.79	0.59	2.61

CV = Coefficient of variation

Note: Variability from some factors may be numerically negative. This can occur if the variability due to those factors is very small. In these cases, SD and CV are shown as 0.00.

## Co-Infection

A co-infection study evaluated the ability of the Aptima CV/TV assay to detect *Candida* species, *C. glabrata*, and *T. vaginalis* when more than one organism is present in the same specimen. Low concentration of one target lysate and high concentration of another target lysate in SVSM were tested in combination. Panel composition and concentrations are listed in Table 22. All testing resulted in 100% detection for both targets present except for the combination of low *C. glabrata* (3X LoD) and high *T. vaginalis* ( $1 \times 10^4$  cells/mL or  $1 \times 10^5$  cells/mL). Further testing was conducted and resulted in 100% detection for the combination of low *C. glabrata* (3X LoD) and high *T. vaginalis* ( $1 \times 10^3$  cells/mL).

Table 22: Co-Infection Panel

Panel Member	<i>C. albicans</i> Concentration	<i>C. glabrata</i> Concentration	<i>T. vaginalis</i> Concentration
<i>C. albicans</i> Low; <i>C. glabrata</i> High	13317 CFU/mL <sup>1</sup>	$1 \times 10^6$ CFU/mL	N/A
<i>C. albicans</i> Low; <i>T. vaginalis</i> High	13317 CFU/mL <sup>1</sup>	N/A	$1 \times 10^5$ cells/mL
<i>C. glabrata</i> Low; <i>T. vaginalis</i> High	N/A	123 CFU/mL <sup>2</sup>	$1 \times 10^3$ cells/mL
<i>C. albicans</i> High; <i>C. glabrata</i> Low	$1 \times 10^6$ CFU/mL	123 CFU/mL <sup>2</sup>	N/A
<i>C. albicans</i> High; <i>T. vaginalis</i> Low	$1 \times 10^6$ CFU/mL	N/A	0.0072 cells/mL <sup>3</sup>
<i>C. glabrata</i> High; <i>T. vaginalis</i> Low	N/A	$1 \times 10^6$ CFU/mL	0.0072 cells/mL <sup>3</sup>

CFU = Colony Forming Units

<sup>1</sup>3X LoD *C. albicans*.

<sup>2</sup>3X LoD *C. glabrata*.

<sup>3</sup>3X LoD *T. vaginalis*.



## Bibliography

1. Hainer BL, Gibson MV. Vaginitis: Diagnosis and Treatment. Am Fam Physician. 2011 Apr 1;83(7):807-15.
2. Granato PA. Vaginitis: Clinical and Laboratory Aspects for Diagnosis. Clinical Microbiology Newsletter. Volume 32, Issue 15, 1 August 2010, Pages 111–116.
3. Achkar JM, Fries BC. Candida infections of the genitourinary tract. Clin Microbiol Rev. 2010 Apr;23(2):253-73.
4. MMWR, Vol. 64, Nr. 3. Sexually transmitted diseases treatment guidelines, June 5, 2015.
5. Fidel PL Jr, Vazquez JA, Sobel JD. Candida glabrata: review of epidemiology, pathogenesis, and clinical disease with comparison to C. albicans. Clin Microbiol Rev. 1999 Jan;12(1):80-96.
6. Mavedzenge SN, Pol BV, Cheng H, Montgomery ET, Blanchard K, de Bruyn G, Ramjee G, Straten Av. Epidemiological synergy of Trichomonas vaginalis and HIV in Zimbabwean and South African women. Sex Transm Dis. 2010 Jul;37(7):460-6.
7. Petrin D, Delgaty K, Bhatt R, Garber G. Clinical and Microbiological Aspects of Trichomonas vaginalis. Clin Microbiol Rev. 1998;11(2):300–317.
8. Clinical and Laboratory Standards Institute. Collection, Transport, Preparation, and Storage of Specimens for Molecular Methods; Approved Guideline. CLSI Document MM13. Wayne, PA; current version.
9. Centers for Disease Control and Prevention/National Institutes of Health. Biosafety in Microbiological and Biomedical Laboratories (BMBL); current version.
10. Clinical and Laboratory Standards Institute. Clinical Laboratory Waste Management. CLSI Document GP5. Villanova, PA; current version.
11. Shew M, et al. Association of condom use, sexual behaviors and sexually transmitted infections with the duration of genital human papillomavirus infection among adolescent women. Arch Pediatr Adolesc Med. 2006;160(2):151-156.
12. Allsworth J, et al. Trichomoniasis and other sexually transmitted infections: results from the 2001-2004 National Health and Nutrition Examination Surveys. Sex Transm Dis. 2009;36(12):738-744.



Hologic, Inc.  
10210 Genetic Center Drive  
San Diego, CA 92121



Hologic BVBA  
Da Vincilaan 5  
1930 Zaventem  
Belgium

Customer Support: +1 800 442 9892  
customersupport@hologic.com

Technical Support: +1 888 484 4747  
molecularsupport@hologic.com

For more contact information visit [www.hologic.com](http://www.hologic.com).

Hologic, Aptima, TMA, Panther, and associated logos are trademarks and/or registered trademarks of Hologic, Inc. and/or its subsidiaries in the United States and/or other countries.

All other trademarks, registered trademarks, and product names that may appear in this package insert are the property of their respective owners.

This product may be covered by one or more U.S. patents identified at [www.hologic.com/patents](http://www.hologic.com/patents).

©2019 Hologic, Inc. All rights reserved.

AW-18812 Rev. 001  
2019-05