

Aptima® Neisseria gonorrhoeae Assay

Instructions for Use
For *in vitro* diagnostic use
For U.S. Export only

General Information 2

Intended Use 2

Summary and Explanation of the Test 2

Principles of the Procedure 3

Summary of Safety and Performance 3

Warnings and Precautions 3

Reagent Storage and Handling Requirements 7

Specimen Collection and Storage 7

Panther System 10

Reagents and Materials Provided 10

Materials Required But Available Separately 11

Optional Materials 12

Panther System Test Procedure 12

Procedural Notes 15

Test Interpretation — QC/Patient Results 17

Limitations 20

Clinical Study Results 22

Expected Values 23

DTS System Clinical Performance 27

Clinical Specimen Agreement 38

Panther System Clinical Specimen Agreement 41

Panther System Clinical Performance 42

Analytical Performance 47

Bibliography 55

Contact Information and Revision History 56

General Information

Intended Use

The Aptima® *Neisseria gonorrhoeae* (GC) assay is a target amplification nucleic acid probe test that utilizes target capture and Transcription Mediated Amplification (TMA™) technology for the *in vitro* qualitative detection of ribosomal RNA (rRNA) from *Neisseria gonorrhoeae* to aid in the diagnosis of gonococcal urogenital disease using the Panther® System. The assay may be used to test the following specimens from symptomatic individuals: clinician-collected endocervical, vaginal and male urethral swab specimens; patient-collected vaginal swab specimens¹ and female and male urine specimens. The assay may be used to test the following specimens from asymptomatic individuals: clinician-collected endocervical and vaginal swab specimens, patient-collected vaginal swab specimens¹ and female and male urine specimens. The assay is also intended for use with the testing of gynecological specimens, from both symptomatic and asymptomatic patients collected in the PreservCyt® Solution.

¹Patient-collected vaginal swab specimens are an option for screening women when a pelvic exam is not otherwise indicated.

Summary and Explanation of the Test

Neisseria gonorrhoeae infections are one of the most common sexually transmitted infections worldwide. In the United States, an estimated 1,568,000 new *N. gonorrhoeae* infections occur each year (1).

N. gonorrhoeae, a non-motile gram-negative diplococcus, is the causative agent of gonorrheal disease. The majority of gonorrheal infections are uncomplicated lower genital tract infections and may be asymptomatic. However, if left untreated in women, infections can ascend and cause pelvic inflammatory disease (PID). PID can manifest as endometritis, salpingitis, pelvic peritonitis, and tubo-ovarian abscesses. A smaller percentage of persons with gonococcal infections may develop Disseminated Gonococcal Infection (DGI) (2, 3).

Conventional diagnosis of GC infection requires isolation of the organism on selective media or the observation of diplococci in Gram stained smears (4). Culture methods can have good clinical sensitivity, but are highly dependent on proper specimen handling. Improper specimen storage and transport can result in the loss of organism viability and yield false negative results. In addition, poor sampling technique, toxic sampling materials, and the inhibition of growth by components of body secretions can also result in false negative results (5, 6). Commonly used non-culture methods for GC detection include direct DNA probe tests and nucleic acid amplification tests (NAATs).

First generation NAATs for GC have technological issues that have limited their performance. These issues include cumbersome specimen processing and specimen inhibition that can yield false negative results (7). The Aptima GC assay is a second generation NAAT that utilizes target capture, TMA, and Hybridization Protection Assay (HPA) technologies to streamline specimen processing, amplify target rRNA, and detect amplicon, respectively. Studies comparing performance and specimen inhibition of various amplification systems have demonstrated the benefits of target capture, TMA, and HPA (8, 9).

According to “Guidance for the detection of gonorrhoea in England”, a 2021 guidance issued by Public Health England, a gonorrhea test should have a minimum positive predictive value (PPV) of 90% in the local setting or patient population (10). If the PPV falls below this threshold a supplementary test should be used to confirm positive test results to improve the

PPV. Supplementary tests are described as a second nucleic acid amplification test (NAAT) performed on the same sample, but which detects a different nucleic acid target sequence. The Aptima GC assay and the Aptima Combo 2® Assay both target the 16S rRNA subunit for capture and detection. The capture oligomer is the same for both assays, but the Aptima GC assay detects a different region of the 16S rRNA subunit than the Aptima Combo 2 assay and thus can be considered a suitable supplementary test to improve the PPV of Aptima Combo 2 testing when recommended by local health guidelines.

Principles of the Procedure

Specimens are collected and transferred into their respective specimen transport tubes. The transport solution in these tubes releases the rRNA target and protects it from degradation during storage. When the Aptima GC assay is performed in the laboratory, the target rRNA molecule is isolated from the specimens by use of a capture oligomer via target capture that utilizes magnetic microparticles. The capture oligomer contains a sequence complementary to a specific region of the target molecule as well as a string of deoxyadenosine residues. During the hybridization step, the sequence specific region of the capture oligomer binds to a specific region of the target molecule. The capture oligomer:target complex is then captured out of solution by decreasing the temperature of the reaction to room temperature. This temperature reduction allows hybridization to occur between the deoxyadenosine region on the capture oligomer and the poly-deoxythymidine molecules that are covalently attached to the magnetic particles. The microparticles, including the captured target molecule bound to them, are pulled to the side of the reaction vessel using magnets and the supernatant is aspirated. The particles are washed to remove residual specimen matrix that may contain amplification reaction inhibitors. After the target capture steps are completed, the specimens are ready for amplification.

Target amplification assays are based on the ability of complementary oligonucleotide primers to specifically anneal and allow enzymatic amplification of the target nucleic acid strands. The Hologic® TMA reaction replicates a specific region of the 16S rRNA from GC via DNA intermediates. A unique set of primers is used for the target molecule. Detection of the rRNA amplification product sequences (amplicon) is achieved using nucleic acid hybridization. A single-stranded chemiluminescent DNA probe, which is complementary to a region of the target amplicon, is labeled with an acridinium ester molecule. The labeled DNA probe combines with amplicon to form stable RNA:DNA hybrids. The Selection Reagent differentiates hybridized from unhybridized probe, eliminating the generation of signal from unhybridized probe. During the detection step, light emitted from the labeled RNA:DNA hybrids is measured as photon signals in a luminometer, and are reported as Relative Light Units (RLU).

Summary of Safety and Performance

The SSP (Summary of Safety and Performance) is available in the European database on medical devices (Eudamed), where it is linked to the device identifiers (Basic UDI-DI). To locate the SSP for Aptima GC assay, refer to the Basic Unique Device Identifier (BUDI): **54200455DIAGAPTGCQL**.

Warnings and Precautions

- A. For *in vitro* diagnostic use.
- B. For professional use.

- C. To reduce the risk of invalid results, carefully read the entire package insert and the *Panther/Panther Fusion® System Operator's Manual* prior to performing the assay.
- D. Only personnel adequately trained in the use of the Aptima GC assay and in handling potentially infectious materials should perform this procedure. If a spill occurs, immediately disinfect following appropriate site procedures.
- E. For additional specific warnings, precautions and procedures to control contamination for the Panther/Panther Fusion system, consult the *Panther/Panther Fusion System Operator's Manual*.

Laboratory Related

- F. Use only supplied or specified disposable laboratory ware.
- G. Use routine laboratory precautions. Do not eat, drink or smoke in designated work areas. Wear disposable, powderless gloves, protective eye wear, and laboratory coats when handling specimens and kit reagents. Wash hands thoroughly after handling specimens and kit reagents.
- H. **Warning: Irritant and Corrosive.** Avoid contact of Auto Detect 2 with skin, eyes and mucous membranes. If this fluid comes into contact with skin or eyes, wash with water. If this fluid spills, dilute the spill with water before wiping dry.
- I. Work surfaces, pipettes, and other equipment must be regularly decontaminated with 2.5% to 3.5% (0.35 M to 0.5 M) sodium hypochlorite solution.
- J. Dispose of all materials that have come into contact with specimens and reagents in accordance with applicable national, international, and regional regulations.
- K. Use good standard practices for molecular laboratories including environmental monitoring. See *Procedural Notes* for suggested Lab Contamination Monitoring Protocol for the Panther system.

Specimen Related



- L. This assay has been tested using endocervical and male urethral swab specimens, PreservCyt solution Pap specimens, vaginal swab specimens, and female and male urine specimens only. Performance with specimens other than those specified under *Specimen Collection and Storage* has not been evaluated.
- M. Expiration dates listed on the collection kits pertain to the collection site and not the testing facility. Samples collected any time prior to the expiration date of the collection kit, and transported and stored in accordance with the package insert, are valid for testing even if the expiration date on the collection tube has passed.
- N. The PreservCyt solution has been validated as an alternative medium for testing with the Aptima GC assay. PreservCyt solution Pap specimens processed with instruments other than the ThinPrep® Processor or other instruments have not been evaluated to test for use in the Aptima GC assay.
- O. After urine has been added in the urine transport tube, the liquid level must fall between the two black indicator lines on the tube label. Otherwise, the specimen must be rejected.

- P. Maintain proper storage conditions during specimen shipping to ensure the integrity of the specimen. Specimen stability under shipping conditions other than those recommended has not been evaluated.
- Q. Specimens may be infectious. Use Universal Precautions when performing this assay. Proper handling and disposal methods should be established by the laboratory director. Only personnel adequately trained in handling infectious materials should be permitted to perform this diagnostic procedure.
- R. Avoid cross-contamination during the specimen handling steps. Specimens can contain extremely high levels of organisms. Ensure that specimen containers from different patients do not contact one another during specimen handling in the laboratory. Change gloves if they come in contact with a specimen.
- S. Discard used materials without passing over any other container.
- T. If the lab receives a swab specimen transport tube with no swab, two swabs, a cleaning swab, or a swab not supplied by Hologic, the specimen must be rejected. Prior to rejecting a swab transport tube with no swab, verify that it is not an Aptima® Specimen Transfer Tube as this specimen transport tube will not contain a swab.
- U. For PreservCyt solution Pap specimens, collect according to the manufacturer's instructions. Aliquots subsequently removed from the PreservCyt vial for testing by the Aptima GC assay should be processed using only the Aptima® Specimen Transfer Kit.
- V. Upon piercing, liquid can discharge from Aptima specimen transport tube caps under certain conditions. Follow instructions in the *Panther System Test Procedure* to prevent this occurrence.

Assay Related

- W. Do not use this kit or controls after its expiration date.
- X. Do not interchange, mix, or combine assay reagents from kits with different lot numbers. Aptima controls and assay fluids can be from different lot numbers.
- Y. Avoid microbial and nuclease contamination of reagents.
- Z. Cap and store reagents at the specified temperatures. The performance of the assay may be affected by use of improperly stored reagents. See *Reagent Storage and Handling Requirements* and *Panther System Test Procedure* for more information.
- AA. Do not combine any assay reagents or fluids without specific instruction. Do not top off reagents or fluids. The Panther system verifies reagent levels.
- AB. Some reagents of this kit are labeled with risk and safety symbols.

Note: Hazard communication reflects the EU Safety Data Sheets (SDS) classifications. For hazard communication information specific to your region, refer to the Safety Data Sheet Library at www.hologic.com/sds. For more information on the symbols, refer to the symbol legend on www.hologic.com/package-inserts.

EU Hazard Information	
—	<p>Amplification Reagent <i>HEPES 25 - 30%</i></p> <p>—</p> <p>H412 - Harmful to aquatic life with long lasting effects. P273 - Avoid release to the environment. P501 - Dispose of contents/container to an approved waste disposal plant.</p>
—	<p>Enzyme Reagent <i>TRITON X-100 1- 5%</i></p> <p>—</p> <p>H402 - Harmful to aquatic life. P273 - Avoid release to the environment. P501 - Dispose of contents/container to an approved waste disposal plant.</p>
—	<p>Probe Reagent <i>LAURYL SULFATE LITHIUM SALT 35 - 40%</i> <i>SUCCINIC ACID 10 - 15%</i></p> <p>—</p> <p>H412 - Harmful to aquatic life with long lasting effects. P273 - Avoid release to the environment. P501 - Dispose of contents/container to an approved waste disposal plant.</p>
—	<p>Enzyme Reconstitution Solution <i>GLYCEROL 20 - 25%</i> <i>TRITON X-100 5 - 10%</i></p> <p>—</p> <p>H402 - Harmful to aquatic life. P273 - Avoid release to the environment. P501 - Dispose of contents/container to an approved waste disposal plant.</p>
 	<p>Selection Reagent <i>BORIC ACID 0 - 10%</i> <i>TRITON X-100 0 - 10%</i> <i>SODIUM HYDROXIDE 0 - 10%</i></p> <p>DANGER</p> <p>H315 - Causes skin irritation H360FD - May damage fertility. May damage the unborn child. P264 - Wash face, hands and any exposed skin thoroughly after handling. P280 - Wear protective gloves/protective clothing/eye protection/face protection. P321 - Specific treatment (see supplemental first aid instructions on the SDS). P201 - Obtain special instructions before use. P202 - Do not handle until all safety precautions have been read and understood. P405 - Store locked up. P501 - Dispose of contents/container to an approved waste disposal plant.</p>
—	<p>Target Capture Reagent <i>HEPES 5 - 10%</i> <i>EDTA 1 - 5%</i> <i>LITHIUM HYDROXIDE, MONOHYDRATE 1 - 5%</i></p> <p>—</p> <p>H401 - Toxic to aquatic life. H412 - Harmful to aquatic life with long lasting effects. P273 - Avoid release to the environment. P501 - Dispose of contents/container to an approved waste disposal plant.</p>

Reagent Storage and Handling Requirements

- A. The following table shows the storage conditions and stability for reagents and controls:

Reagent	Unopened Storage	Open Kit (Reconstituted)	
		Storage	Stability
Amplification Reagent	2°C to 8°C		
Enzyme Reagent	2°C to 8°C		
Probe Reagent	2°C to 8°C		
Target Capture Reagent B	2°C to 8°C		
Amplification Reconstitution Solution	2°C to 30°C	2°C to 8°C	60 days
Enzyme Reconstitution Solution	2°C to 30°C	2°C to 8°C	60 days
Probe Reconstitution Solution	2°C to 30°C	2°C to 8°C	60 days
Selection Reagent	2°C to 30°C	2°C to 30°C	60 days
Target Capture Reagent	15°C to 30°C	15°C to 30°C	60 days
Positive Control	2°C to 8°C		Single Use Vial
Negative Control	2°C to 8°C		Single Use Vial

- B. If the Selection Reagent is stored refrigerated, let it come to room temperature before placing on the Panther system.
- C. The following reagents is stable when stored at 15°C to 30°C (room temperature):
Target Capture Reagent.
- D. Working Target Capture Reagent GC (wTCR) is stable for 60 days when stored at 15°C to 30°C. Do not refrigerate.
- E. After reconstitution, the Enzyme Reagent, Amplification Reagent, and Probe Reagent are stable for 60 days when stored at 2°C to 8°C.
- F. Discard any unused reconstituted reagents and wTCR after 60 days or after the Master Lot expiration date, whichever comes first.
- G. Avoid cross-contamination during reagent handling and storage. Recap all reconstituted reagents with new reagent caps each time prior to storage.
- H. Controls are stable until the date indicated on the vials.
- I. Reagents stored onboard the Panther system have 72 hours of onboard stability
- J. The Probe Reagent and Reconstituted Probe Reagent are photosensitive. Store the reagents protected from light.
- K. Upon warming to room temperature, some control tubes may appear cloudy or contain precipitates. Cloudiness or precipitation associated with controls does not affect control performance. The controls may be used whether they are clear or cloudy/precipitated. If clear controls are desired, solubilization may be expedited by incubating them at the upper end of the room temperature range (15°C to 30°C).
- L. Do not freeze the reagents.

Specimen Collection and Storage

Note: Handle all specimens as if they contain potentially infectious agents. Use Universal Precautions.

Note: Take care to avoid cross-contamination during sample handling steps. For example, discard used material without passing over open tubes.

The Aptima GC assay is designed to detect the presence of GC in clinician-collected endocervical, vaginal and male urethral swab specimens, patient-collected vaginal swab specimens, female and male urine specimens, and PreservCyt solution Pap specimens. Performance with specimens other than those collected with the following specimen collection kits has not been evaluated:

- Aptima Multitest Swab Specimen Collection Kit
- Aptima Urine Collection Kit for Male and Female Urine Specimens
- Aptima Unisex Swab Specimen Collection Kit for Endocervical and Male Urethral Swab Specimens
- Aptima Specimen Transfer Kit (for use with gynecological samples collected in PreservCyt solution)

A. Specimen Collection

Refer to the appropriate specimen collection kit package insert for collection instructions.

B. Specimen Transport and Storage Before Testing

1. Swab Specimens

- a. After collection, transport and store the swab in the specimen transport tube at 2°C to 30°C until tested. Specimens must be assayed with the Aptima GC assay within 60 days of collection. If longer storage is needed, freeze urogenital specimens in the swab specimen transport tube within 7 days of collection at –20°C to –70°C to allow testing for up to 12 months after collection (see *Specimen Stability Studies*).

2. Urine Specimens

- a. Maintain urine specimen at 2°C to 30°C after collection and transfer to the urine specimen transport tube within 24 hours of collection. Transport to the lab in the primary collection container or the transport tube at 2°C to 30°C. Store at 2°C to 30°C and test the processed urine specimens with the Aptima GC assay within 30 days of collection.
- b. If longer storage is needed, freeze urine specimens in the urine specimen transport tube within 7 days of collection at –20°C to –70°C to allow testing up to 12 months after collection (see *Specimen Stability Studies*).

3. PreservCyt Solution Pap Specimens

- a. PreservCyt solution Pap specimens intended for GC testing must be processed for cytology and/or transferred to a specimen transfer tube within 30 days of collection when stored at 2°C to 30°C (see *Specimen Stability Studies*).
- b. If the ThinPrep Aliquot Removal procedure will be used, refer to the *ThinPrep Systems Processor Operator's Manual* for instructions on aliquot removal. Transfer 1 mL of the removed aliquot into a specimen transfer tube according to the instructions in the Aptima Specimen Transfer Kit and Aptima Transfer Solution package insert.
- c. If testing the specimen after processing using the ThinPrep systems processor, process the PreservCyt solution Pap specimen in accordance with the *ThinPrep Systems Processor Operator's Manual* and the Aptima Specimen Transfer Kit and Aptima Transfer Solution package insert. Transfer 1 mL of the fluid remaining in

the PreservCyt solution vial into a specimen transfer tube according to the instructions in the Aptima Specimen Transfer Kit and Aptima Transfer Solution package insert.

- d. Once the PreservCyt solution Pap specimen is transferred to the Aptima specimen transfer tube, the specimen must be assayed with the Aptima GC assay within 30 days when stored at 2°C to 8°C or 14 days when stored at 15°C to 30°C. If longer storage is needed, freeze specimen within 7 days of transfer to the Aptima specimen transfer tube at –20°C to –70°C to allow testing up to 12 months after transfer (see *Specimen Stability Studies*).

C. Specimen Storage After Testing

1. Specimens that have been assayed must be stored upright in a rack.
2. Cover the specimen transport tubes with a new, clean plastic film or foil barrier.
3. If assayed samples need to be frozen or shipped, remove the penetrable caps and place new non-penetrable caps on the specimen transport tubes. If specimens need to be shipped for testing at another facility, recommended temperatures must be maintained. Prior to uncapping previously tested and recapped samples, specimen transport tubes must be centrifuged for 5 minutes at 420 Relative Centrifugal Force (RCF) to bring all of the liquid down to the bottom of the tube. **Avoid splashing and cross-contamination.**

Note: *Specimens must be shipped in accordance with applicable national and international transportation regulations.*

Panther System

Reagents for the Aptima GC assay are listed below for the Panther system. Reagent Identification Symbols are also listed next to the reagent name.

Reagents and Materials Provided

Aptima Neisseria gonorrhoeae Assay Kit, 100 tests (2 boxes and 1 Controls kit) (Cat. No. 302927)

Aptima Neisseria gonorrhoeae Assay Refrigerated Box (Box 1 of 2)
(store at 2°C to 8°C upon receipt)

Symbol	Component	Quantity
A	Amplification Reagent <i>Non-infectious nucleic acids dried in buffered solution containing < 5% bulking agent.</i>	1 vial
E	Enzyme Reagent <i>Reverse transcriptase and RNA polymerase dried in HEPES buffered solution containing < 10% bulking reagent.</i>	1 vial
P	Probe Reagent <i>Non-infectious chemiluminescent DNA probes dried in succinate buffered solution containing < 5% detergent.</i>	1 vial
TCR-B	Target Capture Reagent B <i>Non-infectious nucleic acids in a buffered solution containing < 5% detergent.</i>	1 x 0.30 mL

Aptima Neisseria gonorrhoeae Assay Room Temperature Box (Box 2 of 2)
(store at 15°C to 30°C upon receipt)

Symbol	Component	Quantity
AR	Amplification Reconstitution solution <i>Aqueous solution containing preservatives.</i>	1 x 11.9 mL
ER	Enzyme Reconstitution solution <i>HEPES buffered solution containing a surfactant and glycerol.</i>	1 x 6.3 mL
PR	Probe Reconstitution solution <i>Succinate buffered solution containing < 5% detergent.</i>	1 x 15.2 mL
S	Selection Reagent <i>600 mM borate buffered solution containing surfactant.</i>	1 x 43.0 mL
TCR	Target Capture Reagent <i>Buffered solution containing solid phase and capture oligomers.</i>	1 x 26.0 mL
	Reconstitution Collars	3
	Master Lot Barcode Sheet	1 sheet

Aptima Controls Kit
(store at 2°C to 8°C upon receipt)

Symbol	Component	Quantity
PGC/NCT	Positive Control, GC / Negative Control, CT <i>Non-infectious GC nucleic acid in a buffered solution containing < 5% detergent. Each 400 µL sample contains the estimated rRNA equivalent of 50 GC cells (250 fg/assay*).</i>	5 x 1.7 mL
PCT/NGC	Positive Control, CT/ Negative Control, GC <i>Non-infectious CT nucleic acid in a buffered solution containing < 5% detergent. Each 400 µL sample contains the estimated rRNA equivalent of 1 CT IFU (5 fg/assay*).</i>	5 x 1.7 mL

*The rRNA equivalents were calculated based on the genome size and estimated DNA:RNA ratio/cell of each organism.

Materials Required But Available Separately

Note: Materials available from Hologic have catalog numbers listed, unless otherwise specified.

	<u>Cat. No.</u>
Panther System	303095
Panther Fusion System	PRD-04172
Panther System Continuous Fluid and Waste (Panther Plus)	PRD-06067
Aptima Assay Fluids Kit <i>(Aptima Wash solution, Aptima Buffer for Deactivation Fluid, and Aptima Oil Reagent)</i>	303014 (1000 tests)
Aptima Auto Detect Kit	303013 (1000 tests)
Multi-tube units (MTUs)	104772-02
Panther Waste Bag Kit	902731
Panther Waste Bin Cover	504405
Or Panther Run Kit <i>contains MTUs, waste bags, waste bin covers, assay fluids, and auto detects</i>	303096 (5000 tests)
Tips, 1000 µL filtered, conductive, liquid sensing, and disposable <i>Not all products are available in all regions. Contact your representative for region-specific information</i>	901121 (10612513 Tecan) 903031 (10612513 Tecan) MME-04134 (30180117 Tecan) MME-04128
Aptima Specimen Transfer Kit <i>for use with specimens in PreservCyt Solution</i>	301154C
Aptima Specimen Transfer Kit — printable for use with specimens in PreservCyt Solution	PRD-05110
Aptima Multitest Swab Specimen Collection Kit	PRD-03546
Aptima Unisex Swab Specimen Collection Kit for Endocervical and Male Urethral Swab Specimens	301041
Aptima Urine Specimen Collection Kit for Male and Female Urine Specimens	301040
Aptima Urine Specimen Transport Tubes for Male and Female Urine Specimens	105575

Bleach, 5% to 8.25% (0.7 M to 1.16 M) sodium hypochlorite solution	—
Disposable gloves	—
Aptima penetrable caps	105668
Replacement non-penetrable caps	103036A
Replacement caps for the 100-test kits	—
<i>Amplification, Enzyme, and Probe reagent</i>	
<i>reconstitution solutions</i>	CL0041 (100 caps)
<i>TCR and Selection reagent</i>	501604 (100 caps)

Optional Materials

	<u>Cat. No.</u>
Aptima Controls Kit	301110
Hologic Bleach Enhancer for Cleaning <i>for routine cleaning of surfaces and equipment</i>	302101
Tube Rocker	—
Lint-free Wipes	—
Plastic-backed Bench Covers	—

Panther System Test Procedure

Note: See the Panther/Panther Fusion System Operator's Manual for additional Panther system procedural information.

A. Work Area Preparation

1. Clean work surfaces where reagents and samples will be prepared. Wipe down work surfaces with 2.5% to 3.5% (0.35 M to 0.5 M) sodium hypochlorite solution. Allow the sodium hypochlorite solution to contact surfaces for at least 1 minute and then follow with a water rinse. Do not allow the sodium hypochlorite solution to dry. Cover the bench surface on which the reagents and samples will be prepared with clean, plastic-backed absorbent laboratory bench covers.
2. Clean a separate work surface where samples will be prepared. Use the procedure described above (Step A.1).
3. Clean any pipettors. Use cleaning procedure described above (Step A.1).

B. Reagent Reconstitution/Preparation of a New Kit

Note: Reagent reconstitution should be performed prior to beginning any work on the Panther System.

1. To reconstitute Amplification, Enzyme, and Probe Reagents, combine the bottles of lyophilized reagent with the reconstitution solution. If refrigerated, allow the reconstitution solutions to reach room temperature before use.
 - a. Pair each reconstitution solution with its lyophilized reagent. Ensure that the reconstitution solution and reagent have matching label colors before attaching the reconstitution collar.
 - b. Check the lot numbers on the Master Lot Barcode Sheet to ensure that the appropriate reagents are paired.
 - c. Open the lyophilized reagent glass vial and firmly insert the notched end of the reconstitution collar into the glass vial opening (Figure 1, Step 1).

- d. Open the matching reconstitution solution, and set the cap on a clean, covered work surface.
- e. While holding the reconstitution solution bottle on the bench, firmly insert the other end of the reconstitution collar into the reconstitution solution bottle (Figure 1, Step 2).
- f. Slowly invert the assembled bottles. Allow the solution to drain from the reconstitution solution bottle into the glass vial (Figure 1, Step 3).
- g. Gently swirl the solution in the bottle to mix. Avoid creating foam while swirling the bottle. (Figure 1, Step 4).
- h. Wait for the lyophilized reagent to go into solution, then invert the assembled bottles again, tilting at a 45° angle to minimize foaming (Figure 1, Step 5). Allow all of the liquid to drain back into the reconstitution solution bottle.
- i. Remove the reconstitution collar and glass vial (Figure 1, Step 6).
- j. Recap the reconstitution solution bottle. Record operator initials and the reconstitution date on the label (Figure 1, Step 7).
- k. Discard the collar and vial (Figure 1, Step 8).

Option: Additional mixing of the Amplification, Enzyme and Probe Reagents is allowed by placing recapped plastic bottles on a tube rocker set at a moderate speed and tilt for a minimum of 5 minutes. Ensure reagents are thoroughly mixed.

Warning: Avoid creating foam when reconstituting reagents. Foam compromises the level-sensing in the Panther system.

Warning: Adequate mixing of the reagents is necessary to achieve expected assay results.

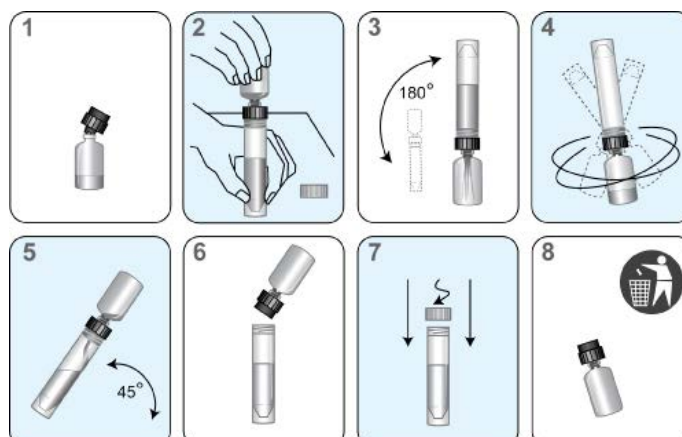


Figure 1. Panther System Reconstitution Process

2. Prepare the working Target Capture Reagent (wTCR)
 - a. Pair the appropriate bottles of TCR and TCR-B.
 - b. Check the reagent lot numbers on the Master Lot Barcode Sheet to make sure that the appropriate reagents in the kit are paired.
 - c. Open the bottle of TCR, and set the cap on a clean, covered work surface.
 - d. Open the bottle of TCR-B and pour the entire contents into the bottle of TCR. Expect a small amount of liquid to remain in the TCR-B bottle.

- e. Cap the bottle of TCR and gently swirl the solution to mix the contents. Avoid creating foam during this step.
 - f. Record operator initials and the current date on the label.
 - g. Discard the TCR-B bottle and cap.
3. Prepare Selection Reagent
- a. Check the lot number on the reagent bottle to make sure that it matches the lot number on the Master Lot Barcode Sheet.
 - b. Record operator initials and the current date on the label.

Note: *Thoroughly mix Amplification, Enzyme, Probe, and Selection Reagents by gently inverting prior to loading on the system. Avoid creating foam during inversion of reagents.*

C. Reagent Preparation for Previously Reconstituted Reagents

1. Previously reconstituted Amplification, Enzyme, and Probe Reagents must reach room temperature (15°C to 30°C) prior to the start of the assay.
Option: *The reconstituted Amplification, Enzyme and Probe Reagents capped plastic bottles may be placed on a tube rocker set at a moderate speed and tilt until reagents reach room temperature and are thoroughly mixed.*
2. If reconstituted Probe Reagent contains precipitate that does not return to solution at room temperature, heat the capped bottle at a temperature that does not exceed 62°C for 1 to 2 minutes. After this heat step, the Probe Reagent may be used even if residual precipitate remains. Mix Probe Reagent by inversion, being careful not to induce foam, prior to loading onto the system.
3. Thoroughly mix each reagent by gently inverting prior to loading on the system. Avoid creating foam during inversion of reagents.
4. Do not top off reagent bottles. The Panther system will recognize and reject bottles that have been topped off.
Warning: *Adequate mixing of the reagents is necessary to achieve expected assay results.*

D. Specimen Handling

1. Allow the controls and specimens to reach room temperature prior to processing.
2. Do not vortex specimens.
3. Visually confirm that each specimen tube meets one of the following criteria.
 - a. The presence of a single blue Aptima collection swab in a unisex swab specimen transport tube.
 - b. The presence of a single pink Aptima collection swab in a multitest or vaginal swab specimen transport tube.
 - c. A final volume of urine between the black fill lines of a urine specimen transport tube.
 - d. The absence of a swab in the Aptima specimen transport tube for PreservCyt solution Pap specimens.
4. Inspect specimen tubes before loading into the rack.
 - a. If a specimen tube contains bubbles in the space between the liquid and the cap, centrifuge the tube for 5 minutes at 420 RCF to eliminate the bubbles.

- b. If a specimen tube has a lower volume than typically observed when collection instructions have been followed, centrifuge the tube for 5 minutes at 420 RCF to ensure that no liquid is in the cap.
- c. If the liquid level in a urine specimen tube is not between the two black indicator lines on the label, the specimen must be rejected. Do not pierce an overfilled tube.
- d. If a urine specimen tube contains precipitate, heat the specimen at 37°C for up to 5 minutes. If the precipitate does not go back into solution, visually ensure that the precipitate does not prevent delivery of the specimen.

Note: Failure to follow Steps 4a–c may result in liquid discharge from the specimen tube cap.

Note: Up to 4 separate aliquots can be tested from each specimen tube. Attempts to pipette more than 4 aliquots from the specimen tube can lead to processing errors.

E. System Preparation

1. Set up the system according to the instructions in the *Panther/Panther Fusion System Operator's Manual* and *Procedural Notes*. Make sure that the appropriately sized reagent racks and TCR adapters are used.
2. Load samples.

Procedural Notes

A. Controls

1. To work properly with the Aptima assay software for the Panther system, one pair of controls is required. The Positive Control, CT / Negative Control, GC and the Positive Control, GC / Negative Control CT tubes can be loaded in any rack position or in any Sample Bay Lane on the Panther system. Patient specimen pipetting will begin when one of the following two conditions has been met:
 - a. A pair of controls is currently being processed by the system.
 - b. Valid results for the controls are registered on the system.
2. Once the control tubes have been pipetted and are processing for a specific reagent kit, patient specimens can be run with the associated assay reagent kit up to 24 hours **unless**:
 - a. Controls results are invalid.
 - b. The associated assay reagent kit is removed from the system.
 - c. The associated assay reagent kit has exceeded stability limits.
3. Each Aptima control tube can be tested once. Attempts to pipette more than once from the tube can lead to processing errors.

B. Temperature

Room temperature is defined as 15°C to 30°C.

C. Glove Powder

As in any reagent system, excess powder on some gloves may cause contamination of opened tubes. Powderless gloves are recommended.

D. Lab Contamination Monitoring Protocol for the Panther system

There are many laboratory-specific factors that may contribute to contamination, including testing volume, workflow, disease prevalence and various other laboratory activities. These factors should be taken into consideration when contamination monitoring frequency is being established. Intervals for contamination monitoring should be established based on each laboratory's practices and procedures.

To monitor for laboratory contamination, the following procedure may be performed using the Aptima unisex swab specimen collection kit for endocervical and male urethral swab specimens:

1. Label swab transport tubes with numbers corresponding to the areas to be tested.
2. Remove the specimen collection swab (blue shaft swab with green printing) from its packaging, wet the swab in Aptima Specimen Transport Medium (STM), and swab the designated area using a circular motion.
3. Immediately insert the swab into transport tube.
4. Carefully break the swab shaft at the score line; use care to avoid splashing of the contents.
5. Recap the swab transport tube tightly.
6. Repeat Steps 2 to 5 for each area to be swabbed.
7. Test samples with the Aptima GC assay on the Panther system.
8. Further investigation should be performed if any samples yield a positive result.

If the results are GC positive or equivocal, see *Test Interpretation — QC/Patient Results*. For additional Panther system-specific contamination monitoring information, contact Hologic Technical Support.

Test Interpretation — QC/Patient Results

A. Test Interpretation

Assay test results are automatically interpreted by the Aptima assay software using the GC protocol. A test result may be negative, equivocal, positive, or invalid as determined by total RLU in the detection step (see below). A test result may be invalid due to RLU values outside the normal expected ranges. Initial equivocal and invalid test results should be retested.

Test Interpretation	Total RLU (x1000)
Negative	0* to < 50
Equivocal	50 to < 100
Low RLU Positive ^{1,2}	100 to < 2,000
Positive ¹	2,000 to < 12,000
Invalid	0* or > 12,000

*A zero (0 x 1000) RLU result on the run report represents a value between zero and 999 RLU. RLU values less than 690 on the Panther system will be reported as invalid.

¹Refer to Table 3 for RLU distribution of results. The magnitude of RLU is not indicative of the level of organism in the specimen.

²In the low positive range, data suggest positive results should be interpreted carefully, with the understanding that the likelihood of a false positive may be higher than a true positive.

B. Quality Control Results and Acceptability

The Negative Control for GC, which is labeled “CONTROL + CT PCT / CONTROL – GC NGC,” and the Positive Control for GC, which is labeled “CONTROL + GC PGC / CONTROL – CT NCT,” act as controls for the target capture, amplification, and detection steps of the assay. In accordance with guidelines or requirements of local, state, and/or federal regulations or accrediting organizations, additional controls for cell lysis and RNA stabilization may be included. The Positive Control for GC, which is labeled “CONTROL + GC PGC / CONTROL – CT NCT” contains non-infectious GC rRNA. If desired, additional controls can be ordered as a kit. Correct preparation of specimens is confirmed visually by the presence of a single Aptima collection swab in a specimen transport tube, a final volume of urine in between the black fill lines of a urine specimen transport tube, or the absence of a swab in an Aptima specimen transfer tube for liquid Pap specimens.

The Positive Controls must produce the following test results:

Control	Total RLU (x1000)	GC Result
Positive Control, CT / Negative Control, GC	0* and < 50	Negative
Positive Control, GC / Negative Control, CT	≥ 100 and < 12,000	Positive

*A zero (0 x 1000) RLU result on the run report represents a value between zero and 999 RLU. RLU values less than 690 on the Panther system will be reported as invalid.

1. The Aptima assay software automatically evaluates the controls according to the above criteria and will report the Run Status as PASS if the run control criteria are met, and FAIL if the run control criteria are not met.
2. If the Run Status is FAIL, all test results in the same run are invalid and must not be reported.
3. Each laboratory should implement appropriate control procedures to satisfy local requirements.

Note: Contact Hologic Technical Support for help with out-of-range controls.

4. Negative Controls may not be effective in monitoring random carryover. See *Carryover Studies for the Panther System* for results from a high-target analytical carryover study that was performed to demonstrate control of carryover on the Panther system.

C. Specimen Preparation Control (optional)

The Negative Control for GC, which is labeled “CONTROL + CT PCT / CONTROL – GC NGC,” and the Positive Control for GC, which is labeled “CONTROL + GC PGC / CONTROL – CT NCT,” act as controls for the target capture, amplification, and detection steps of the assay and must be included in each assay run. If desired, controls for cell lysis and RNA stabilization can be tested in accordance with the requirements of appropriate accrediting organizations or individual laboratory procedures. Known positive specimens can serve as controls by being prepared and tested in conjunction with unknown specimens. Specimens used as preparation controls must be stored, handled, and tested according to the package insert. Specimen preparation controls should be interpreted in the same manner as described for patient test specimens. See *Test Interpretation — QC/Patient Results* and/or *Patient Test Results*.

D. Patient Test Results

1. If the controls in any run do not yield the expected results, test results on patient specimens in the same run must not be reported.
2. Swab, urine, and PreservCyt solution Pap specimen results. See *Notes* below.
 - a. Initial results

GC Pos*	Positive for GC rRNA.
GC Neg	Presumed negative for GC rRNA.
GC Equiv	Sample should be retested.
Invalid	Sample should be retested.

b. Retest results

GC Pos*	Positive for GC rRNA.
GC Neg	Presumed negative for GC rRNA.
GC Equiv	Indeterminate, a new specimen should be collected.
Invalid	Indeterminate, a new specimen should be collected.

*Low RLU Positive specimen results are included in this category. See *Test Interpretation — QC/Patient Results* above.

Notes

- The first valid, non-equivocal result for each analyte is the result that should be reported.
- Careful consideration of performance data is recommended for interpreting Aptima GC test results for asymptomatic individuals or any individuals in low prevalence populations.
- A negative result does not preclude the presence of a GC infection because results are dependent on adequate specimen collection, absence of inhibitors, and sufficient rRNA to be detected. Test results may be affected by improper specimen collection, improper specimen storage, technical error, specimen mix-up, or target levels below the assay limit of detection.
- Testing of an endocervical specimen is recommended for female patients who are clinically suspected of having a chlamydial or gonococcal infection. If both a Pap and endocervical swab are collected, the PreservCyt solution Pap specimen must be collected before the endocervical swab specimen.

Limitations

- A. Use of this assay is limited to personnel who have been trained in the procedure. Failure to follow the instructions given in this package insert may result in erroneous results.
- B. The effects of tampon use, douching, and specimen collection variables have not been assessed for their impact on the detection of GC.
- C. The presence of mucus in endocervical specimens does not interfere with the detection of GC by the Aptima GC assay. However, to ensure proper endocervical sampling, excess mucus should be removed.
- D. Urine, vaginal swab, and PreservCyt solution Pap specimen sampling is not designed to replace cervical exams and endocervical specimens for diagnosis of female urogenital infections. Patients may have cervicitis, urethritis, urinary tract infections, or vaginal infections due to other causes or concurrent infections with other agents.
- E. The Aptima GC assay is not intended for the evaluation of suspected sexual abuse or for other medico-legal indications.
- F. Reliable results are dependent on adequate specimen collection. Because the transport system used for this assay does not permit microscopic assessment of specimen adequacy, proper specimen collection techniques are necessary. Refer to package insert of the appropriate Aptima specimen collection kit.
- G. Therapeutic failure or success cannot be determined with the Aptima GC assay since nucleic acid may persist following appropriate antimicrobial therapy.
- H. Results from the Aptima GC assay should be interpreted in conjunction with other laboratory and clinical data available to the clinician.
- I. A negative result does not preclude a possible infection because results are dependent on adequate specimen collection. Test results may be affected by improper specimen collection, technical error, specimen mix-up, or target levels below the assay limit of detection.
- J. The Aptima GC assay provides qualitative results. Therefore, a correlation cannot be drawn between the magnitude of a positive assay signal and the number of organisms in a specimen.
- K. For the vaginal swab, endocervical swab, male urethral swab and urine specimen clinical studies, performance for detecting GC is derived from high prevalence populations. Positive results in low prevalence populations should be interpreted carefully with the understanding that the likelihood of a false positive may be higher than a true positive.
- L. For the PreservCyt solution Pap specimen clinical studies, the Aptima GC assay performance for detecting GC is derived primarily from low prevalence populations. Nonetheless, positive results in low prevalence populations should be interpreted carefully with the understanding that the likelihood of a false positive may be higher than a true positive.
- M. Performance of the Aptima specimen transfer kit was not evaluated for testing the same PreservCyt solution Pap specimen both before and after ThinPrep Pap processing.

- N. PreservCyt solution Pap specimens processed with instruments other than the ThinPrep 2000 processor have not been evaluated for use in Aptima assays.
- O. Patient-collected vaginal swab specimens are an option for screening women when a pelvic exam is not otherwise indicated.
- P. The patient-collected vaginal swab specimen application is limited to health care facilities where support/counseling is available to explain the procedures and precautions.
- Q. The Aptima GC assay has not been validated for use with vaginal swab specimens collected by patients at home.
- R. The performance of the Aptima GC assay has not been evaluated in adolescents less than 14 years of age.
- S. Testing of urethral swab specimens from asymptomatic males is not recommended because of the low predictive value of a positive result observed in the clinical study.
- T. The performance of the Panther system has not been evaluated at altitudes above 2000 m (6561 feet).
- U. There is no evidence of degradation of nucleic acids in PreservCyt solution. If a PreservCyt solution Pap specimen has small numbers of GC cellular material, uneven distribution of this cellular material may occur. Also, when compared to direct sampling with STM, the additional volume of PreservCyt solution results in greater dilution of the sample material. These factors may affect the ability to detect small numbers of organisms in the collected material. If negative results from the specimen do not fit with the clinical impression, a new specimen may be necessary.
- V. Customers must independently validate an LIS transfer process.

Clinical Study Results

The performance characteristics of the Aptima GC assay were established in three clinical investigations conducted in North America. The first clinical investigation established the sensitivity, specificity, and predictive values of the Aptima GC assay using clinician-collected endocervical, vaginal, and male urethral swab specimens, patient-collected vaginal swab specimens, and male and female urine specimens. The second clinical investigation established the sensitivity, specificity, and predictive values of the Aptima GC assay using PreservCyt transport medium (component of the ThinPrep 2000 system). PreservCyt solution Pap specimens were also evaluated for within-laboratory precision with the Aptima GC assay.

The initial clinical investigations to establish the sensitivity, specificity and predictive values of the Aptima GC assay were completed using a semi-automated DTS® system. The assay was then migrated to a fully automated Tigris® DTS system (without any changes to assay formulation) using clinical comparability studies. Lastly, clinical comparability studies were used to migrate the Aptima GC assay from Tigris DTS to its current system of use, the Panther system. Data from the initial studies using the DTS or Tigris DTS systems may be shown herein to support establishment of the assay performance, although current use of these systems is no longer supported by the manufacturer.

In the third clinical investigation, the clinical performance of the Aptima GC assay was evaluated in sexually active male and female subjects at least 14 years of age with or without symptoms of STIs. This study evaluated patient-collected vaginal swab and urine specimens tested using the Panther system.

Expected Values

The positivity of GC in patient populations depends on risk factors such as age, lifestyle, the presence or absence of symptoms, and the sensitivity of the test used to detect infections. A summary of the positivity of GC in North America, by specimen type as determined by the Aptima GC assay using the DTS system is shown in Table 1a and Table 1b for two clinical investigations. Table 1c summarizes positivity of *N. gonorrhoeae* for the Aptima GC assay on the Panther system as determined by an additional clinical investigation.

Table 1a: Positivity of *N. gonorrhoeae* by Clinical Site and Overall as Determined by Aptima GC Assay Results on the DTS System.

Site	% (#positive/#tested)											
	MS		MU		FS		FU		PVS		CVS	
1	21.4	(54/252)	21.4	(54/252)	6.1	(14/229)	5.7	(13/230)	6.4	(14/219)	6.1	(14/230)
2	26.5	(93/351)	20.1	(71/354)	16.1	(32/199)	15.0	(30/200)	16.2	(32/198)	16.6	(33/199)
3	0.0	(0/4)	0.0	(0/4)	4.4	(5/114)	3.5	(4/113)	3.6	(4/111)	3.5	(4/113)
4	N/A		N/A		2.3	(6/266)	1.9	(5/270)	2.2	(6/267)	3.0	(8/269)
5	5.5	(11/200)	5.5	(11/200)	1.5	(3/199)	1.0	(2/199)	1.0	(2/199)	1.0	(2/199)
6	14.5	(44/304)	13.4	(41/305)	8.2	(24/294)	5.7	(17/296)	8.3	(24/290)	7.5	(22/295)
7	5.8	(12/207)	5.8	(12/207)	0.0	(0/102)	0.0	(0/102)	0.0	(0/102)	0.0	(0/102)
8	N/A		N/A		2.0	(1/49)	2.0	(1/49)	2.1	(1/48)	2.0	(1/51)
All	16.2	(214/1318)	14.3	(189/1322)	5.9	(85/1452)	4.9	(72/1459)	5.8	(83/1434)	5.8	(84/1458)

MS = Male Urethral Swab; **MU** = Male Urine; **FS** = Female Endocervical Swab; **FU** = Female Urine; **PVS** = Patient-Collected Vaginal Swab; **CVS** = Clinician-Collected Vaginal Swab; **N/A** = not available.

Table 1b: Positivity of *N. gonorrhoeae* by Clinical Site and Overall as Determined by Aptima GC Assay Results on the DTS System Using PreservCyt Solution Pap Solution Specimens

Site	% (#positive/#tested)	
1	5.0	(5/100)
2	0.8	(1/124)
3	0.8	(4/475)
4	1.4	(4/287)
5	0.0	(0/297)
6	0.5	(2/364)
All	1.0	(16/1647)

Table 1c: Positivity of *N. gonorrhoeae* as Determined by Aptima GC Assay Results on the Panther System in Patient-collected Vaginal Swab, Female Urine, and Male Urine Samples by Clinical Site

Site	Positivity % (# positive/# tested with valid non-equivocal results)		
	PVS	FU	MU
1	14.3 (3/21)	13.6 (3/22)	21.7 (38/175)
2	1.3 (5/383)	1.3 (5/385)	0.8 (3/373)
3	0 (0/75)	0 (0/74)	0 (0/61)
4	0 (0/5)	0 (0/5)	0 (0/13)
5	2.0 (5/254)	2.0 (5/250)	8.3 (34/409)
6	2.0 (10/494)	2.1 (10/484)	9.4 (29/307)
7	2.0 (5/246)	1.6 (4/245)	5.3 (12/225)
8	0 (0/95)	0 (0/97)	0 (0/32)
9	0.3 (1/313)	0 (0/261)	0 (0/218)
10	4.3 (11/255)	4.0 (10/253)	11.0 (10/91)
11	0 (0/96)	0 (0/91)	0 (0/54)
All	1.8 (40/2237)	1.7 (37/2167)	6.4 (126/1958)

FU = female urine; MU = male urine; PVS = patient-collected vaginal swab.

Positive and Negative Predictive Values for Hypothetical Prevalence Rates in North America

The estimated positive and negative predictive values (PPV and NPV) for different hypothetical prevalence rates using the Aptima GC assay on the DTS system are shown in Table 2a. These calculations are based on hypothetical prevalence rates and the overall sensitivity and specificity estimated from the patient infected status. The overall sensitivity and specificity for the Aptima GC assay on the DTS system are 97.6% and 99.3%, respectively (Table 2a). The actual PPV and NPV for clinician-collected endocervical, vaginal and male urethral swab, patient-collect vaginal swab, and male and female urine specimens are shown in Table 6a for each clinical site and overall. The actual PPV and NPV for PreservCyt solution Pap specimens using the Aptima GC assay on the DTS system are shown in Table 6b.

Table 2a: Positive and Negative Predictive Values for Hypothetical Prevalence Rates in North America on the DTS System

Hypothetical Prevalence Rate (%)	Sensitivity (%)	Specificity (%)	PPV (%)	NPV (%)
1	97.6	99.3	58.7	100.0
2	97.6	99.3	74.1	100.0
5	97.6	99.3	88.1	99.9
10	97.6	99.3	94.0	99.7
15	97.6	99.3	96.1	99.6
20	97.6	99.3	97.2	99.4
25	97.6	99.3	97.9	99.2
30	97.6	99.3	98.4	99.0

The estimated PPV and NPV of the Aptima GC assay on the Panther system across different hypothetical prevalence rates are shown for each specimen type in Table 2b. For each specimen type, the PPV and NPV are derived for different hypothetical prevalence

rates using the overall sensitivity and specificity estimates from the multi-center clinical study (see Table 11).

Table 2b: Positive and Negative Predictive Values for Hypothetical Prevalence Rates in North America on the Panther System

Specimen Type		Hypothetical Prevalence						
		1%	2%	5%	10%	15%	20%	25%
PVS	PPV (%)	91.3	95.5	98.2	99.1	99.5	99.6	99.7
	NPV (%)	99.9	99.9	99.7	99.4	99.1	98.8	98.4
FU	PPV (%)	95.2	97.6	99.0	99.5	99.7	99.8	99.8
	NPV (%)	99.9	99.8	99.6	99.2	98.7	98.1	97.5
MU	PPV (%)	94.8	97.4	99.0	99.5	99.7	99.8	99.8
	NPV (%)	100	100	99.9	99.8	99.7	99.6	99.5

FU = female urine; MU = male urine; NPV = negative predictive value; PPV = positive predictive value; PVS = patient-collected vaginal swab.

Aptima GC Assay on the DTS System RLU Distribution

Figure 2 shows the RLU distribution for the Aptima GC assay for the following specimen types tested in the clinical study: from symptomatic subjects, clinician-collected endocervical, vaginal, and male urethral swab specimens and patient-collected female and male urine specimens; and from asymptomatic subjects, clinician-collected endocervical and vaginal swab specimens and patient-collected vaginal swab, female and male urine specimens. Table 3 summarizes the RLU distribution for the total positive and total negative results, as well as the false positive and false negative results for these specimen types relative to infected patient status. Across certain specimen types, there is a trend toward an increasing proportion of true positives as the RLU values increase.

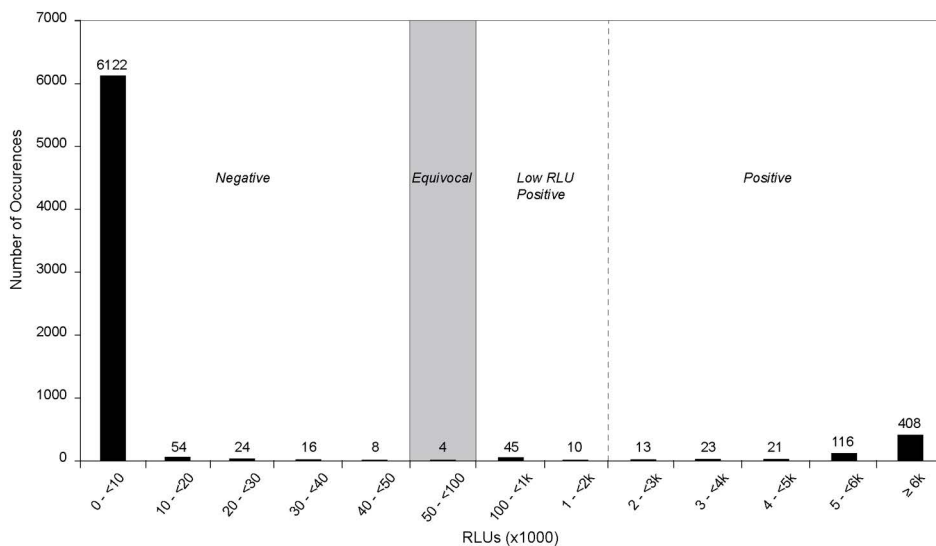


Figure 2. Frequency of RLU Distribution for the Aptima GC Assay on the DTS System

Table 3: Aptima GC Assay RLU Distribution on the DTS System

	RLUs (x 1000)												
	0 – <10	10 – <20	20 – <30	30 – <40	40 – <50	50 – <100	100 – <1000	1000 – <2000	2000 – <3000	3000 – <4000	4000 – <5000	5000 – <6000	≥6000
Total Positives	-	-	-	-	-	-	45	10	13	23	21	116	408
Total False Positives	-	-	-	-	-	-	35	6	2	4	0	3	0
CVS	-	-	-	-	-	1	5	3	0	1	0	2	0
PVS	-	-	-	-	-	0	2	0	0	1	0	1	0
FS	-	-	-	-	-	2	12	1	0	0	0	0	0
MS	-	-	-	-	-	1	9	0	1	0	0	0	0
FU	-	-	-	-	-	0	2	0	0	1	0	0	0
MU	-	-	-	-	-	0	5	2	1	1	0	0	0
Total Negatives	6122	54	24	16	8	-	-	-	-	-	-	-	-
Total False Negatives	7	2	1	2	1	-	-	-	-	-	-	-	-
CVS	2	0	0	0	0	-	-	-	-	-	-	-	-
PVS	0	0	0	0	0	-	-	-	-	-	-	-	-
FS	0	0	0	1	1	-	-	-	-	-	-	-	-
MS	0	1	0	0	0	-	-	-	-	-	-	-	-
FU	3	1	1	1	0	-	-	-	-	-	-	-	-
MU	2	0	0	0	0	-	-	-	-	-	-	-	-

CVS = clinician-collected vaginal swab; **PVS** = patient-collected vaginal swab from asymptomatic subjects only; **FS** = female endocervical swab; **MS** = male urethral swab from symptomatic subjects only; **FU** = female urine; **MU** = male urine.

Shaded column denotes equivocal zone.

DTS System Clinical Performance

Endocervical Swab, Male Urethral Swab, Vaginal Swab, and Urine Specimen Clinical Specimen Study

Clinician-collected endocervical, vaginal and male urethral swab, patient-collected vaginal swab, and male and female urine specimens were collected from 2,787 symptomatic and asymptomatic, male and female subjects attending OB/GYN, sexually transmitted disease (STD), teen, and family planning clinics at eight geographically diverse clinical sites in North America. Subjects were classified as symptomatic if symptoms such as discharge, dysuria, and pelvic pain were reported by the subject. Subjects were classified as asymptomatic if the subject did not report symptoms. Of the 1,392 asymptomatic subjects enrolled in the study, 2 were less than 16 years of age, 237 were between the ages of 16 and 20, 423 were between the ages of 21 and 25, and 730 were greater than 25 years of age. Of the 1,395 symptomatic subjects enrolled in the study, 211 were between the ages of 16 and 20, 494 were between the ages of 21 and 25, and 690 were greater than 25 years of age.

Three specimens were collected from each of the 1,322 eligible male subjects. Five specimens were collected from each of the 1,465 eligible female subjects. For male subjects, two randomized urethral swabs were collected followed by one urine specimen. For female subjects, one urine specimen was collected followed by one patient-collected vaginal swab, one clinician-collected vaginal swab, and two randomized endocervical swabs. Aptima GC assay and Aptima Combo 2 assay GC results were generated from the two vaginal swabs, one endocervical swab, one male urethral swab, and a male and female urine aliquot. The remaining endocervical swab, male urethral swab, and a male and female urine aliquot were tested using another commercially-available NAAT. Endocervical and male urethral swab specimens and male and female urine specimens tested in the Aptima Combo 2 assay and the other commercially available NAAT were used as the reference NAATs to determine infected status for each subject. Specimen testing was conducted either at the site of subject enrollment or at an external testing site.

All performance calculations were based on the total number of Aptima GC assay results for clinician-collected endocervical, vaginal and male urethral swab, and male and female urine specimens compared to a patient infected status algorithm for each gender. In the algorithm, the designation of a subject as being infected or not infected with GC was based on swab and urine specimen results from the commercially-available Aptima Combo 2 assay and the other commercially-available NAAT. Subjects were considered infected with GC if two of the four swab and urine specimens tested positive in the Aptima Combo 2 assay and the other reference NAAT (one specimen testing positive in each NAAT). Subjects were considered non-infected if less than two reference NAAT results were positive. Culture was not used as a reference test.

A total of 7,653 Aptima GC assay results (using the DTS system) were used to calculate sensitivity and specificity. Sensitivity and specificity for GC by gender, specimen type and symptom status, as appropriate, are presented in Table 4. Table 6a shows the Aptima GC assay sensitivity, specificity, and predictive values compared to patient infected status for each clinical site and overall. Tables 7a-7e summarize the number of results from symptomatic and asymptomatic subjects designated as infected or non-infected with GC according to the patient infected status algorithm.

Of the 2,787 subjects enrolled, there were 15 subjects with unknown GC patient infected status. Subjects were designated with an unknown patient infected status if results were missing that prevented conclusive determination of infected status. These subjects' results were not included in any performance calculations. Of the 7,704 Aptima GC assay results,

there were 22 specimens (0.29%) that initially produced invalid or equivocal assay results. Upon retesting these specimens, 4 remained equivocal and were excluded from the analyses. The remaining 18 specimens produced valid test results upon retesting and were used in the clinical performance calculations.

Table 4: Sensitivity and Specificity of the Aptima GC Assay Relative to Patient Infected Status by Symptom Status and Overall for Male Urethral Swab, Male Urine, Female Endocervical Swab, Female Urine, Asymptomatic Patient-Collected Vaginal Swab and Clinician-Collected Vaginal Swab

Specimen	Symptom Status	N	TP	FP	TN	FN	Sensitivity (95% CI)	Specificity (95% CI)	
Male	Swab	Symptomatic	575	171	10 ^a	393	1	99.4 (96.8–100)	97.5 (95.5–98.8)
	Urine	Symptomatic	576	171	4 ^b	400	1	99.4 (96.8–100)	99.0 (97.5–99.7)
		Asymptomatic	745	9	5 ^c	730	1	90.0 (55.5–99.7)	99.3 (98.4–99.8)
		All	1321	180	9 ^d	1130	2	98.9 (96.1–99.9)	99.2 (98.5–99.6)
Female	Swab	Symptomatic	805	52	8 ^e	744	1	98.1 (89.9–100)	98.9 (97.9–99.5)
		Asymptomatic	635	20	5 ^f	609	1	95.2 (76.2–99.9)	99.2 (98.1–99.7)
		All	1440	72	13 ^g	1353	2	97.3 (90.6–99.7)	99.0 (98.4–99.5)
	Urine	Symptomatic	810	48	2 ^h	755	5	90.6 (79.3–96.9)	99.7 (99.0–100)
		Asymptomatic	639	21	1 ⁱ	616	1	95.5 (77.2–99.9)	99.8 (99.1–100)
		All	1449	69	3 ^j	1371	6	92.0 (83.4–97.0)	99.8 (99.4–100)
Patient-Collected	Vaginal Swab	Asymptomatic	629	21	4 ^k	604	0	100 (83.9–100)	99.3 (98.3–99.8)
Clinician-Collected	Vaginal Swab	Symptomatic	809	52	7 ^m	749	1	98.1 (89.9–100)	99.1 (98.1–99.6)
		Asymptomatic	637	21	4 ⁿ	611	1	95.5 (77.2–99.9)	99.3 (98.3–99.8)
		All	1446	73	11 ^o	1360	2	97.3 (90.7–99.7)	99.2 (98.6–99.6)

TP = true positive; FP = false positive; TN = true negative; FN = false negative; CI = confidence interval.

Aptima Combo 2 Assay GC results: # positive results / # specimens tested ^a2/10; ^b1/4; ^c1/5; ^d2/9; ^e5/8; ^f2/5; ^g7/13; ^h1/2; ⁱ1/1; ^j2/3; ^k3/4; ^l8/11; ^m6/7; ⁿ3/4; ^o9/11.

PreservCyt Solution Pap Specimen Clinical Specimen Study

A prospective multi-center clinical study was conducted to evaluate the use of the PreservCyt transport medium as an alternative medium for gynecological specimens for the detection of *N. gonorrhoeae* by the Aptima GC assay. One thousand six hundred forty-seven (1,647) symptomatic and asymptomatic subjects attending OB/GYN, family planning, public health, women's, and STD clinics were enrolled and evaluated in the clinical study. Of these subjects, 1,288 were asymptomatic subjects and 359 were symptomatic subjects (Table 7e). Subjects were enrolled from sites with GC prevalence that ranged from 0.0% to 5.0% (Table 6b).

Two specimens were collected from each eligible subject: one PreservCyt solution Pap specimen and one endocervical swab specimen. PreservCyt solution Pap specimens were collected with the spatula/cyto-brush or a broom-like brush cervical sampling device. The distribution of cervical sampling devices is summarized in Table 5a by specimen collection site and overall.

PreservCyt solution Pap specimens were processed in accordance with the ThinPrep 2000 Processor Operator's Manual and Aptima Specimen Transfer Kit and Aptima Transfer Solution package insert. After processing the PreservCyt solution Pap specimen with the

ThinPrep 2000 Processor, the specimen was transferred into the Aptima specimen transfer kit for testing with the Aptima GC assay.

Sensitivity and specificity of the Aptima GC assay in PreservCyt solution Pap specimens were calculated by comparing results to the patient infected status. The algorithm included Aptima Combo 2 assay and Aptima GC assay results in endocervical swab specimens. Both reference NAATs were required to be positive to establish an infected patient status. At least one reference NAAT was required to be negative to establish a non-infected patient status. The one equivocal result that was obtained from a reference NAAT was considered to be discordant with the investigative assay for the purpose of calculating performance, and thus the patient infected status was categorized as non-infected (n=1). Table 7e summarizes the frequency of test outcomes for the endocervical swab specimens tested with the Aptima Combo 2 assay and Aptima GC assay.

Table 5b shows the sensitivities and specificities of the Aptima GC assay by symptom status and overall. Overall sensitivity was 92.3% (12/13). In symptomatic and asymptomatic subjects, sensitivities were 100% (7/7) and 83.3% (5/6), respectively. Overall specificity was 99.8% (1630/1634). In symptomatic and asymptomatic subjects, specificities were 99.4% (350/352) and 99.8% (1280/1282), respectively.

Table 6b shows the sensitivities and specificities of the Aptima GC assay by specimen collection site and overall. Sensitivities ranged from 80.0% to 100%. Specificities ranged from 99.0% to 100%.

Table 5a: Distribution of Cervical Sampling Device Used for PreservCyt Solution Pap Specimens

Cervical Sampling Device Used	Clinical Collection Site						Total
	1	2	3	4	5	6	
Spatula/Cytobrush	0	124	475	287	57	364	1307
Broom-Type Device	100	0	0	0	240	0	340

Table 5b: Sensitivity and Specificity of the Aptima GC Assay Relative to Patient Infected Status by Symptom Status and Overall for PreservCyt Solution Pap Specimen

Symptom	Aptima GC PreservCyt Solution Result	+/+	+/-	-/+	-/-	Sensitivity (%) (95% CI)	Specificity (%) (95% CI)
Symptomatic	Positive	7	0	0	2	100 (7/7) (59.0–100)	99.4 (350/352) (98.0–99.9)
	Negative	0	0	0	350		
	Total	7	0	0	352		
Asymptomatic	Positive	5	0	1 ¹	1	83.3 (5/6) (35.9–99.6)	99.8 (1280/1282) (99.4–100)
	Negative	1	0	5	1275		
	Total	6	0	6	1276		
All	Positive	12	0	1	3	92.3 (12/13) (64.0–99.8)	99.8 (1630/1634) (99.4–99.9)
	Negative	1	0	5	1625		
	Total	13	0	6	1628		

CI = confidence interval.

+/+ = Positive endocervical swab specimen result in the Aptima Combo 2 Assay/Positive endocervical swab specimen result in the Aptima GC Assay.

+/- = Positive endocervical swab specimen result in the Aptima Combo 2 Assay/Negative endocervical swab specimen result in the Aptima GC Assay.

-/+ = Negative endocervical swab specimen result in the Aptima Combo 2 Assay/Positive endocervical swab specimen result in the Aptima GC Assay.

-/- = Negative endocervical swab specimen result in the Aptima Combo 2 Assay/Negative endocervical swab specimen result in the Aptima GC Assay.

¹One specimen had a discordant result: Equivocal endocervical swab specimen result in the Aptima Combo 2 Assay/Positive endocervical swab specimen result in the Aptima GC Assay.

Table 6a: Sensitivity, Specificity, and Predictive Values of the Aptima GC Assay Relative to Patient Infected Status by Clinical Site and Overall for Male Urethral Swab, Male Urine, Female Endocervical Swab, Female Urine, Asymptomatic Patient-Collected Vaginal Swab, and Clinician-Collected Vaginal Swab

Specimen	Site	N	TP	FP	TN	FN	Prev (%)	Sensitivity (95% CI)	Specificity (95% CI)	PPV (%)	NPV (%)	
Swab	1	145	49	0	96	0	33.8	100 (92.7–100)	100 (96.2–100)	100	100	
	2	177	66	8	102	1	37.9	98.5 (92.0–100)	92.7 (86.2–96.8)	89.2	99.0	
	3	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	
	4	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	
	5	49	7	1	41	0	14.3	100 (59.0–100)	97.6 (87.4–99.9)	87.5	100	
	6	150	37	1	112	0	24.7	100 (90.5–100)	99.1 (95.2–100)	97.4	100	
	7	54	12	0	42	0	22.2	100 (73.5–100)	100 (91.6–100)	100	100	
	8	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	
	All	575	171	10	393	1	29.9	99.4 (96.8–100)	97.5 (95.5–98.8)	94.5	99.7	
Male	Urine	1	252	53	1	198	0	21.0	100 (93.3–100)	99.5 (97.2–100)	98.1	100
		2	353	68	3	280	2	19.8	97.1 (90.1–99.7)	98.9 (96.9–99.8)	95.8	99.3
		3	4	0	0	4	0	0.0	N/A	100 (39.8–100)	N/A	100
		4	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A
		5	200	8	3	189	0	4.0	100 (63.1–100)	98.4 (95.5–99.7)	72.7	100
		6	305	39	2	264	0	12.8	100 (91.0–100)	99.2 (97.3–99.9)	95.1	100
		7	207	12	0	195	0	5.8	100 (73.5–100)	100 (98.1–100)	100	100
		8	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A
		All	1321	180	9	1130	2	13.8	98.9 (96.1–99.9)	99.2 (98.5–99.6)	95.2	99.8

Table 6a: Sensitivity, Specificity, and Predictive Values of the Aptima GC Assay Relative to Patient Infected Status by Clinical Site and Overall for Male Urethral Swab, Male Urine, Female Endocervical Swab, Female Urine, Asymptomatic Patient-Collected Vaginal Swab, and Clinician-Collected Vaginal Swab (continued)

Specimen	Site	N	TP	FP	TN	FN	Prev (%)	Sensitivity (95% CI)	Specificity (95% CI)	PPV (%)	NPV (%)
Swab	1	226	12	2	212	0	5.3	100 (73.5–100)	99.1 (96.7–99.9)	85.7	100
	2	197	29	3	164	1	15.2	96.7 (82.8–99.9)	98.2 (94.8–99.6)	90.6	99.4
	3	114	4	1	109	0	3.5	100 (39.8–100)	99.1 (95.0–100)	80.0	100
	4	260	5	1	254	0	1.9	100 (47.8–100)	99.6 (97.8–100)	83.3	100
	5	199	2	1	196	0	1.0	100 (15.8–100)	99.5 (97.2–100)	66.7	100
	6	294	19	5	269	1	6.8	95.0 (75.1–99.9)	98.2 (95.8–99.4)	79.2	99.6
	7	102	0	0	102	0	0.0	N/A	100 (96.4–100)	N/A	100
	8	48	1	0	47	0	2.1	100 (2.5–100)	100 (92.5–100)	100	100
	All	1440	72	13	1353	2	5.1	97.3 (90.6–99.7)	99.0 (98.4–99.5)	84.7	99.9
Female Urine	1	227	11	2	213	1	5.3	91.7 (61.5–99.8)	99.1 (96.7–99.9)	84.6	99.5
	2	198	30	0	167	1	15.7	96.8 (83.3–99.9)	100 (97.8–100)	100	99.4
	3	113	4	0	109	0	3.5	100 (39.8–100)	100 (96.7–100)	100	100
	4	265	5	0	260	0	1.9	100 (47.8–100)	100 (98.6–100)	100	100
	5	199	2	0	197	0	1.0	100 (15.8–100)	100 (98.1–100)	100	100
	6	296	16	1	275	4	6.8	80.0 (56.3–94.3)	99.6 (98.0–100)	94.1	98.6
	7	102	0	0	102	0	0.0	N/A	100 (96.4–100)	N/A	100
	8	49	1	0	48	0	2.0	100 (2.5–100)	100 (92.6–100)	100	100
	All	1449	69	3	1371	6	5.2	92.0 (83.4–97.0)	99.8 (99.4–100)	95.8	99.6
Patient-Collected Vaginal Swab (Asymptomatic)	1	70	5	1	64	0	7.1	100 (47.8–100)	98.5 (91.7–100)	83.3	100
	2	46	7	1	38	0	15.2	100 (59.0–100)	97.4 (86.5–99.9)	87.5	100
	3	45	2	0	43	0	4.4	100 (15.8–100)	100 (91.8–100)	100	100
	4	152	1	0	151	0	0.7	100 (2.5–100)	100 (97.6–100)	100	100
	5	130	1	0	129	0	0.8	100 (2.5–100)	100 (97.2–100)	100	100
	6	75	5	2	68	0	6.7	100 (47.8–100)	97.1 (90.1–99.7)	71.4	100
	7	68	0	0	68	0	0.0	N/A	100 (94.7–100)	N/A	100
	8	43	0	0	43	0	0.0	N/A	100 (91.8–100)	N/A	100
	All	629	21	4	604	0	3.3	100 (83.9–100)	99.3 (98.3–99.8)	84.0	100
Clinician-Collected Vaginal Swab	1	227	12	2	213	0	5.3	100 (73.5–100)	99.1 (96.7–99.9)	85.7	100
	2	197	30	3	163	1	15.7	96.8 (83.3–99.9)	98.2 (94.8–99.6)	90.9	99.4
	3	113	4	0	109	0	3.5	100 (39.8–100)	100 (96.7–100)	100	100
	4	263	5	3	255	0	1.9	100 (47.8–100)	98.8 (96.6–99.8)	62.5	100
	5	199	2	0	197	0	1.0	100 (15.8–100)	100 (98.1–100)	100	100
	6	295	19	3	272	1	6.8	95.0 (75.1–99.9)	98.9 (96.8–99.8)	86.4	99.6
	7	102	0	0	102	0	0.0	N/A	100 (96.4–100)	N/A	100
	8	50	1	0	49	0	2.0	100 (2.5–100)	100 (92.7–100)	100	100
	All	1446	73	11	1360	2	5.2	97.3 (90.7–99.7)	99.2 (98.6–99.6)	86.9	99.9

TP = true positive; FP = false positive; TN = true negative; FN = false negative; Prev = prevalence; CI = confidence interval; PPV = positive predictive value; NPV = negative predictive value; NA = not available.

Table 6b: Sensitivity, Specificity and Predictive Values of the Aptima GC Assay Relative to Patient Infected Status by Clinical Site and Overall for PreservCyt Solution Pap Specimens

Site	Aptima GC PreservCyt Solution Result	+/+	+/-	-/+	-/-	Prev (%)	Sensitivity (%) (95% CI)	Specificity (%) (95% CI)	PPV(%)	NPV(%)
1	Positive	5	0	0	0	5.0	100 (5/5) (47.8–100)	100 (95/95) (96.2–100)	100	100
	Negative	0	0	0	95					
	Total	5	0	0	95					
2	Positive	1	0	0	0	0.8	100 (1/1) (2.5–100)	100 (123/123) (97.0–100)	100	100
	Negative	0	0	0	123					
	Total	1	0	0	123					
3	Positive	4	0	0	0	1.1	80.0 (4/5) (28.4–99.5)	100 (470/470) (99.2–100)	100	99.8
	Negative	1	0	0	470					
	Total	5	0	0	470					
4	Positive	1	0	0	3	0.3	100 (1/1) (2.5–100)	99.0 (283/286) (97.0–99.8)	25.0	100
	Negative	0	0	3	280					
	Total	1	0	3	283					
5	Positive	0	0	0	0	0.0	N/A	100 (297/297) (98.8–100)	N/A	100
	Negative	0	0	0	297					
	Total	0	0	0	297					
6	Positive	1	0	1 ¹	0	0.3	100 (1/1) (2.5–100)	99.7 (362/363) (98.5–100)	50.0	100
	Negative	0	0	2	360					
	Total	1	0	3	360					
ALL	Positive	12	0	1	3	0.8	92.3 (12/13) (64.0–99.8)	99.8 (1630/1634) (99.4–99.9)	75.0	99.9
	Negative	1	0	5	1625					
	Total	13	0	6	1628					

CI = confidence interval; N/A = not applicable; PPV = positive predictive value; NPV = negative predictive value.

+/+ = Positive endocervical swab specimen result in the Aptima Combo 2 Assay/Positive endocervical swab specimen result in the Aptima GC Assay.

+/- = Positive endocervical swab specimen result in the Aptima Combo 2 Assay/Negative endocervical swab specimen result in the Aptima GC Assay.

-/+ = Negative endocervical swab specimen result in the Aptima Combo 2 Assay/Positive endocervical swab specimen result in the Aptima GC Assay.

-/- = Negative endocervical swab specimen result in the Aptima Combo 2 Assay/Negative endocervical swab specimen result in the Aptima GC Assay.

¹One specimen had a discordant result: Equivocal endocervical swab specimen result in the Aptima Combo 2 Assay/Positive endocervical swab specimen result in the Aptima GC Assay.

Table 7a: Symptomatic Male Urethral Swab Results from Subjects Infected or Non-Infected with *N. gonorrhoeae* According to Patient Infected Status

Patient Infected Status	NAAT 1 (Aptima Combo 2 Assay)		NAAT 2		Aptima GC Assay	Total
	MS	MU	MS	MU	MS	
Infected	+	+	+	+	+	164
Infected	+	+	+	+	-	1
Infected	+	+	+	-	+	3
Infected	+	+	=	+	+	1
Infected	+	-	+	+	+	2
Infected	+	-	+	-	+	1
Non-infected	+	-	-	-	+	2
Non-infected	+	-	-	-	-	1
Non-infected	-	+	-	-	+	1
Non-infected	-	-	+	-	-	1
Non-infected	-	-	-	+	-	2
Non-infected	-	-	-	-	+	3
Non-infected	-	-	-	-	+	2
Non-infected	-	-	-	-	-	386
Non-infected	-	-	-	-	=	1
Non-infected	-	-	-	N/A	-	1
Non-infected	-	-	-	=	-	1
Non-infected	-	-	=	-	-	1
Non-infected	=	-	-	-	+	2
Total						576

N/A = specimen not obtained or available for testing; MS = symptomatic male urethral swab; MU = male urine. The equal symbol (=) represents equivocal or indeterminate on repeat testing.

Table 7b: Male Urine Results from Subjects Infected or Non-Infected with *N. gonorrhoeae* According to Patient Infected Status

Patient Infected Status	NAAT 1 (Aptima Combo 2 Assay)		NAAT 2		Aptima GC Assay	Symptom Status		Total
	MS	MU	MS	MU	MU	Sym	Asym	
Infected	+	+	+	+	+	164	8	172
Infected	+	+	+	+	+	1	0	1
Infected	+	+	+	-	+	3	1	4
Infected	+	+	=	+	+	1	0	1
Infected	+	-	+	+	+	2	0	2
Infected	+	-	+	-	-	1	1	2
Non-infected	+	+	-	-	+	0	1	1
Non-infected	+	-	-	-	-	2	13	15
Non-infected	+	-	-	-	-	1	0	1
Non-infected	-	+	-	-	+	1	0	1
Non-infected	-	+	-	-	-	0	1	1
Non-infected	-	-	+	-	-	1	1	2
Non-infected	-	-	-	+	-	2	2	4
Non-infected	-	-	-	-	+	3	1	4
Non-infected	-	-	-	-	-	2	1	3
Non-infected	-	-	-	-	+	0	3	3
Non-infected	-	-	-	-	-	386	691	1077
Non-infected	-	-	-	-	-	1	2	3
Non-infected	-	-	-	N/A	-	1	4	5
Non-infected	-	-	-	=	-	1	4	5
Non-infected	-	-	=	-	-	1	1	2
Non-infected	-	=	-	-	-	0	1	1
Non-infected	N/A	-	-	-	-	0	1	1
Non-infected	=	-	-	-	-	2	6	8
Non-infected	=	-	-	-	-	0	2	2
Total						576	745	1321

Sym = symptomatic; **Asym** = asymptomatic; **MS** = male urethral swab; **MU** = male urine; **N/A** = specimen not obtained or available for testing.

The equal symbol (=) represents equivocal or indeterminate on repeat testing.

Table 7c: Female Endocervical Swab and Urine Results from Subjects Infected or Non-Infected with *N. gonorrhoeae* According to Patient Infected Status

Patient Infected Status	NAAT 1 (Aptima Combo 2 Assay)		NAAT 2		Aptima GC Assay		Symptom Status		Total
	FS	FU	FS	FU	FS	FU	Sym	Asym	
Infected	+	+	+	+	+	+	43	16	59
Infected	+	+	+	+	+	-	2	0	2
Infected	+	+	+	-	+	+	2	1	3
Infected	+	+	+	-	+	-	0	1	1
Infected	+	+	+	N/A	+	+	1	0	1
Infected	+	+	-	+	+	+	1	1	2
Infected	+	+	-	-	+	+	1	1	2
Infected	+	-	+	+	+	-	1	0	1
Infected	+	-	+	-	+	+	0	1	1
Infected	+	-	+	-	+	-	2	0	2
Infected	-	+	+	+	-	+	1	0	1
Infected	-	+	-	+	-	+	0	1	1
Infected	-	+	-	+	=	+	0	1	1
Infected	-	-	+	+	-	-	1	0	1
Non-infected	+	-	-	-	+	-	4	1	5
Non-infected	+	-	-	-	-	-	1	0	1
Non-infected	-	+	-	-	-	-	1	0	1
Non-infected	-	-	+	-	+	-	1	0	1
Non-infected	-	-	+	-	-	-	5	2	7
Non-infected	-	-	-	+	-	-	2	2	4
Non-infected	-	-	-	-	+	-	1	2	3
Non-infected	-	-	-	-	-	+	1	0	1
Non-infected	-	-	-	-	-	-	718	589	1307
Non-infected	-	-	-	-	=	-	1	0	1
Non-infected	-	-	-	N/A	-	-	2	3	5
Non-infected	-	-	-	=	-	-	11	11	22
Non-infected	-	-	=	-	-	-	1	1	2
Non-infected	-	N/A	-	-	-	N/A	1	1	2
Non-infected	N/A	-	-	-	N/A	-	5	4	9
Non-infected	=	-	-	-	+	-	1	1	2
Total							811	640	1451

Sym = symptomatic; **Asym** = asymptomatic; **FS** = female endocervical swab; **FU** = female urine; **N/A** = specimen not obtained or available for testing.

The equal symbol (=) represents equivocal or indeterminate on repeat testing.

Table 7d: Vaginal Swab Results from Subjects Infected or Non-Infected with *N. gonorrhoeae* According to Patient Infected Status

Patient Infected Status	NAAT 1 (Aptima Combo 2 Assay)		NAAT 2		Aptima GC Assay		Symptom Status		Total
	FS	FU	FS	FU	PVS	CVS	Sym	Asym	
Infected	+	+	+	+	+	+	43	15	58
Infected	+	+	+	+	-	+	1	0	1
Infected	+	+	+	+	-	-	1	0	1
Infected	+	+	+	+	N/A	+	0	1	1
Infected	+	+	+	-	+	+	2	2	4
Infected	+	+	+	N/A	+	+	1	0	1
Infected	+	+	-	+	+	+	1	1	2
Infected	+	+	-	-	+	+	1	1	2
Infected	+	-	+	+	+	+	1	0	1
Infected	+	-	+	-	+	+	2	1	3
Infected	-	+	+	+	+	+	1	0	1
Infected	-	+	-	+	+	+	0	1	1
Infected	-	+	-	+	+	-	0	1	1
Infected	-	-	+	+	-	-	1	0	1
Non-infected	+	-	-	-	-	-	5	1	6
Non-infected	-	+	-	-	-	-	1	0	1
Non-infected	-	-	+	-	+	+	1	0	1
Non-infected	-	-	+	-	-	-	5	2	7
Non-infected	-	-	-	+	+	+	0	1	1
Non-infected	-	-	-	+	-	-	2	1	3
Non-infected	-	-	-	-	+	+	2	1	3
Non-infected	-	-	-	-	+	-	3	1	4
Non-infected	-	-	-	-	-	+	3	1	4
Non-infected	-	-	-	-	-	-	696	577	1273
Non-infected	-	-	-	-	-	N/A	0	1	1
Non-infected	-	-	-	-	-	=	0	1	1
Non-infected	-	-	-	-	N/A	-	16	9	25
Non-infected	-	-	-	-	N/A	N/A	1	0	1
Non-infected	-	-	-	N/A	-	-	2	2	4
Non-infected	-	-	-	N/A	N/A	-	0	1	1
Non-infected	-	-	-	=	-	-	11	10	21
Non-infected	-	-	-	=	-	N/A	0	1	1
Non-infected	-	-	=	-	-	-	1	1	2
Non-infected	-	N/A	-	-	-	-	0	1	1
Non-infected	-	N/A	-	-	N/A	N/A	1	0	1
Non-infected	N/A	-	-	-	-	-	5	4	9
Non-infected	=	-	-	-	-	-	1	1	2
Total							811	640	1451

Sym = symptomatic; **Asym** = asymptomatic; **FS** = female endocervical swab; **FU** = female urine; **PVS** = patient-collected vaginal swab; **CVS** = clinician-collected vaginal swab; **N/A** = specimen not obtained or available for testing.
The equal symbol (=) represents equivocal or indeterminate on repeat testing.

Table 7e: PreservCyt Solution Clinical Study (Patient Infected Status Results from Endocervical Swab Specimens)

Patient Infected Status	Endocervical Swab		Symptom Status	
	Aptima Combo 2 Assay	Aptima GC Assay	Symptomatic	Asymptomatic
Infected	Positive	Positive	7	6
Non-Infected	Negative	Negative	352	1276
Non-Infected	Negative	Positive	0	5
Non-Infected	Equivocal	Positive	0	1
Total			359	1288

RLU Distribution of Aptima Controls

The distribution of the RLUs for the Positive Control, GC / Negative Control, CT and the Positive Control, CT / Negative Control, GC from all the Aptima GC assay runs performed during the clinical specimen study is presented in Table 8.

Table 8: Distribution of RLU of the Aptima Controls During the Clinical Specimen Studies Including Endocervical, Vaginal and Male Urethral Swab, Male and Female Urine Specimens, and PreservCyt Solution Pap Studies

Control	Statistics	RLU (x1000)	
		Swab and Urine Specimen Clinical Study	PreservCyt Solution Pap Specimen Clinical Study
Positive Control, GC / Negative Control, CT	N	193	218
	Mean	5048	4561
	SD	1071	1295
	Maximum	6765	6791
	75 th Percentile	5763	5450
	Median	5175	4859
	25 th Percentile	4645	3804
	Minimum	229	158
Positive Control, CT / Negative Control, GC	N	193	218
	Mean	2.15	2.60
	SD	2.20	2.80
	Maximum	20	29
	75 th Percentile	2	3
	Median	2	2
	25 th Percentile	1	2
	Minimum	0	1

RLU = relative light units; SD = standard deviation.

Note: The RLU value reported by the software was the bases for analysis. The reported RLU value is the total measured RLU divided by 1000 with the digits after the decimal point truncated.

Clinical Specimen Agreement

The Aptima GC Assay was first launched on semi-automated DTS systems and then the Tigris DTS system. In 2010, indications were expanded to use the Aptima GC assay on the Panther system. The Panther system is an alternative, smaller instrument platform to the Tigris DTS system. Both systems are intended to fully automated amplified nucleic acid testing of diagnostics assays. Select assay performance testing completed on the semi-automated DTS systems and Tigris DTS system were leveraged to support assay performance on the Panther system.

Sensitivity, specificity, and predictive values of the Aptima GC assay were established using the DTS system. Agreement between Aptima GC assay results generated on the fully automated Tigris DTS system and semi-automated DTS systems was evaluated by testing endocervical swab, male urethral swab, male and female urine, vaginal swab, and PreservCyt solution Pap specimens. Each of the clinical specimens was tested individually with the Aptima GC assay on both the Tigris DTS system and DTS systems at Hologic. The order of testing was not randomized. Specimens identified for inclusion were tested on the Tigris DTS system followed by testing on DTS systems.

Clinical Specimen Agreement Study — Endocervical Swab, Male Urethral Swab, Female and Male Urine, Vaginal Swab, and PreservCyt Solution Pap Specimens

Female and male subjects attending STD, family planning, and OB/GYN clinics from eight geographically diverse sites with low to high prevalence for GC contributed endocervical swab, male urethral swab, male and female urine, vaginal swab, and PreservCyt solution Pap specimens. The specimens were transferred directly to Hologic for testing. At Hologic, endocervical swab, male urethral swab, male and female urine specimens were first screened with Aptima Combo 2 assay on the Tigris DTS system. The vaginal swab and PreservCyt solution Pap specimens were screened with the Aptima Combo 2 assay on the DTS systems. Specimens with final invalid or equivocal results were not selected in the Aptima GC Clinical Specimen Agreement Study.

One hundred twenty-nine female swabs (70 endocervical and 59 vaginal), 133 male urethral swab, 72 female urine, 130 male urine, and 51 PreservCyt solution Pap specimens with Aptima Combo 2 assay GC positive and negative results were selected for comparison testing between the Tigris DTS system and the DTS systems for the Aptima GC assay. The majority of specimens (88 female swabs, 93 male swab, 47 female urine, 70 male urine, and 34 PreservCyt solution Pap specimens) included for comparison testing were from symptomatic individuals. Specimens with initial invalid or equivocal results were retested using the same system on which the result was generated. Three female urine, 1 vaginal swab, and 1 male urethral swab specimens had initial equivocal results on the DTS systems, upon retest, all had valid results. One male and 1 female urine specimen had initial invalid results on the Tigris DTS system, upon retest, both results were valid.

Table 9 shows the positive, negative, and overall agreements for all paired results for each specimen type by symptomatic status. Female swab specimens (endocervical and vaginal swabs combined), are imbalanced relative to positive and negative samples from symptomatic subjects, but overall agreement for symptomatic subjects was 100%, for asymptomatic subjects was 97.6% (40/41), and for 'all' (symptomatic and asymptomatic combined) overall agreement was 99.2% (128/129). For male urethral swab specimens, overall agreement for symptomatic, asymptomatic, and 'all' subjects was 100%. For female urine specimens, overall agreement for symptomatic subjects was 100%, for asymptomatic subjects was 96.0% (24/25), and 'all' was 98.6% (71/72).

For male urine specimens, overall agreement for symptomatic subjects was 98.6% (69/70), for asymptomatic subjects was 100%, and 'all' was 99.2% (129/130). For PreservCyt solution Pap specimens, overall agreement for symptomatic, asymptomatic, and 'all' subjects was 100%. Because of the relatively smaller specimen number from asymptomatic subjects, these findings may not be generalizable to Aptima GC Tigris DTS system testing with specimens from asymptomatic subjects.

Refer to Table 4 for Aptima GC assay performance estimates for endocervical swab, vaginal swab, male urethral swab, and male and female urine specimens and to Table 5b for PreservCyt solution Pap specimens tested on the DTS systems. Clinical performance estimates for the Tigris DTS system with endocervical swab, vaginal swab, male urethral swab, male and female urine, and PreservCyt solution Pap specimens would be expected to be similar given the agreement findings.

Table 9: Clinical Specimen Agreement Study: Positive, Negative, and Overall Agreements by Symptom Status

Symptom	Specimen	Gender	n	DTS+ Tigris+	DTS+ Tigris-	DTS- Tigris+	DTS- Tigris-	Positive % Agreement (95% CI)	Negative % Agreement (95% CI)	Overall % Agreement (95% CI)
Sym	Swab	Female ¹	88	55	0	0	33	100 (93.5–100)	100 (89.4–100)	100 (95.9–100)
		Male	93	66	0	0	27	100 (94.6–100)	100 (87.2–100)	100 (96.1–100)
	Urine	Female	47	24	0	0	23	100 (85.8–100)	100 (85.2–100)	100 (92.5–100)
		Male	70	60	1	0	9	98.4 (91.2–100)	100 (66.4–100)	98.6 (92.3–100)
	PreservCyt Solution	Female	34	28	0	0	6	100 (87.7–100)	100 (54.1–100)	100 (89.7–100)
	Asym	Swab	Female ¹	41	23	0	1 ²	17	100 (85.2–100)	94.4 (72.7–99.9)
Male			40	7	0	0	33	100 (59.0–100)	100 (89.4–100)	100 (91.2–100)
Urine		Female	25	9	0	1	15	100 (66.4–100)	93.8 (69.8–99.8)	96.0 (79.6–99.9)
		Male	60	5	0	0	55	100 (47.8–100)	100 (93.5–100)	100 (94.0–100)
PreservCyt Solution		Female	17	12	0	0	5	100 (73.5–100)	100 (47.8–100)	100 (80.5–100)

Sym = symptomatic; **Asym** = asymptomatic; **CI** = confidence interval.

“+” denotes a positive result; “-” a negative result.

¹Endocervical and Vaginal Swab samples combined.

²One disagreement in Vaginal Swab.

Table 9: Clinical Specimen Agreement Study: Positive, Negative, and Overall Agreements by Symptom Status

Symptom	Specimen	Gender	n	DTS+ Tigris+	DTS+ Tigris-	DTS- Tigris+	DTS- Tigris-	Positive % Agreement (95% CI)	Negative % Agreement (95% CI)	Overall % Agreement (95% CI)
All	Swab	Female ¹	129	78	0	1 ²	50	100 (95.4–100)	98.0 (89.6–100)	99.2 (95.8–100)
		Male	133	73	0	0	60	100 (95.1–100)	100 (94.0–100)	100 (97.3–100)
	Urine	Female	72	33	0	1	38	100 (89.4–100)	97.4 (86.5–99.9)	98.6 (92.5–100)
		Male	130	65	1	0	64	98.5 (91.8–100)	100 (94.4–100)	99.2 (95.8–100)
	PreservCyt Solution	Female	51	40	0	0	11	100 (91.2–100)	100 (71.5–100)	100 (93.0–100)

Sym = symptomatic; **Asym** = asymptomatic; **CI** = confidence interval.

“+” denotes a positive result; “-” a negative result.

¹Endocervical and Vaginal Swab samples combined.

²One disagreement in Vaginal Swab.

Panther System Clinical Specimen Agreement

Urine was selected as a representative sample type to determine equivalence between the Aptima GC assay on the Tigris DTS and Panther systems, given that urine produces the most variable results of all specimen types intended for use with the Aptima GC assay. Therefore, high agreement among urine specimens would indicate that high agreement could be expected for all other specimen types.

Panels were generated using urine clinical specimens: negative panel members were created using individual urine specimens negative for GC and positive panel members were created using individual naturally-infected GC-positive urine specimens that were diluted with individual gender-matched urine specimens to meet target RLU ranges. Panels were run at three testing sites (two external and in-house).

Table 10: Agreement between Tigris DTS and Panther Systems using Urine Panels

Panther System	Tigris System			
	Negative	Equivocal	Low Positive	Positive
Negative	360	0	0	0
Equivocal	0	0	0	0
Low Positive	0	0	120	9
Positive	0	0	18	198
Total	360	0	138	207
Agreement (%)	100 (360/360)	0 (0/0)	92.2 (318/345)	
95% CI ¹	(96.9–100)	—	(85.8–95.8)	

¹Calculated using the Score method based on the unique number of samples tested.

Negative agreement between the Tigris DTS and Panther systems was 100% for all GC-negative samples. When categorized by RLU range, positive agreement was 92.2%, however the Aptima GC assay on both the Tigris DTS and Panther systems correctly identified all GC-positive panel members as positive. Therefore, agreement between Tigris DTS and Panther systems for qualitative detection of GC in urine specimens was 100%. As the intended use of the Aptima GC assay is the qualitative detection of GC in clinical specimens, assay performance between the two systems can be concluded to be similar.

Refer to Table 4 for Aptima GC assay performance estimates for endocervical, clinician-collected vaginal, and male urethral swabs and to Table 5b for PreservCyt solution Pap specimens tested on the DTS systems. Clinical performance estimates for the Panther system with all specimen types would be expected to be similar given the agreement findings of both the Tigris DTS agreement studies and the Panther system agreement study.

Panther System Clinical Performance

Clinical Study

A prospective, multicenter clinical study was conducted to establish the clinical performance characteristics of the Aptima GC assay on the Panther system. Specimens were collected from 4413 symptomatic and asymptomatic women and men enrolled at 11 geographically and ethnically diverse US clinical sites, including obstetrics and gynecology, family planning, and STI clinics. Subjects were classified as symptomatic if symptoms were reported by the subject. Subjects were classified as asymptomatic if the subject did not report symptoms. One hundred ninety (190) enrolled subjects were not evaluable (28 were withdrawn and 162 did not have at least one specimen with a valid non-excluded Aptima result and a conclusive infected status). Of the 4223 evaluable subjects, 2264 were women and 1959 were men. The average age among evaluable study subjects was 34.5 years (range = 14 to 84 years). Symptoms were reported in 45.6% (1927/4223) of the evaluable subjects.

Up to 5 specimens were collected from each female subject (1 first-catch urine, 4 patient-collected vaginal swab, in that order) and 1 first-catch urine specimen was collected from each male subject. All specimens were collected by the subject at the clinical sites.

Specimens were tested with the Aptima GC assay on the Panther system. Specimens with initial equivocal or invalid Aptima GC assay results or instrument processing errors were retested, volume permitting; valid retest results were included in the performance analyses. Patient-collected vaginal swabs and male and female urine specimens were tested with up to 3 FDA-cleared NAATs to establish the specimen-specific patient infected status (PIS) as follows:

- Male urine PIS was derived from male urine specimens
- Female urine PIS was derived from female urine specimens
- Vaginal swab PIS was derived from vaginal swab and female urine specimens

Performance of the Aptima GC assay was estimated relative to the specimen-specific PIS for each of the specimen types.

Of the specimens collected, 6556 were processed in valid Aptima GC assay runs, including 218 (3.3%) that had to be retested due to initial invalid results. Overall, 6513 (99.3%) had final valid results, and 43 (0.7%) had final invalid results and were excluded from the analyses. A total of 6362 specimens from 4222 evaluable subjects were included in the analyses comparing Aptima GC assay results to the PIS: 2237 patient-collected vaginal swab, 2167 female urine, and 1958 male urine specimens. Four specimens with final GC equivocal results were excluded from the performance analyses.

Performance Results

Performance characteristics of the Aptima GC assay were estimated for each specimen type. Table 11 shows the sensitivity, specificity, PPV, and NPV of the Aptima GC assay on the

Panther system and the prevalence of *N. gonorrhoeae* (based on the specimen-specific PIS) in each specimen type by symptom status and overall.

Table 11: Performance Characteristics of the Aptima GC Assay Female Patient-collected Vaginal Swab, and Male and Female Urine Specimens by Symptom Status

Specimen Type	Symptom Status	n	TP	FP ¹	TN	FN ²	Prev %	Sensitivity % (95% CI) ³	Specificity % (95% CI) ³	PPV % (95% CI) ⁴	NPV % (95% CI) ⁴
PVS	Sym	1086	24	1 ^a	1060	1 ^a	2.3	96.0 (80.5, 99.3)	99.9 (99.5, 100)	96.0 (81.7, 99.9)	99.9 (99.5, 100)
	Asym	1151	14	1 ^b	1135	1 ^b	1.3	93.3 (70.2, 98.8)	99.9 (99.5, 100)	93.3 (72.6, 99.8)	99.9 (99.6, 100)
	All	2237	38	2	2195	2	1.8	95.0 (83.5, 98.6)	99.9 (99.7, 100)	95.0 (84.5, 99.6)	99.9 (99.7, 100)
FU	Sym	1043	25	0	1018	0	2.4	100 (86.7, 100)	100 (99.6, 100)	100 (87.2, 100)	100 (99.7, 100)
	Asym	1124	11	1 ^c	1109	3 ^c	1.2	78.6 (52.4, 92.4)	99.9 (99.5, 100)	91.7 (66.0, 99.7)	99.7 (99.4, 100)
	All	2167	36	1	2127	3	1.8	92.3 (79.7, 97.3)	100 (99.7, 100)	97.3 (87.2, 99.9)	99.9 (99.6, 100)
MU	Sym	825	105	1 ^d	717	2 ^d	13.0	98.1 (93.4, 99.5)	99.9 (99.2, 100)	99.1 (95.1, 100)	99.7 (99.0, 100)
	ASym	1133	20	0	1113	0	1.8	100 (83.9, 100)	100 (99.7, 100)	100 (84.4, 100)	100 (99.7, 100)
	All	1958	125	1	1830	2	6.5	98.4 (94.4, 99.6)	99.9 (99.7, 100)	99.2 (95.8, 100)	99.9 (99.6, 100)

Sym = asymptomatic; Asym = asymptomatic; TP = true positive; FP = false positive; TN = true negative; FN = false negative; Prev = prevalence; CI = confidence interval; PVS = patient-collected vaginal swab; FU = female urine; MU = male urine; PPV = positive predictive value; NPV = negative predictive value.

¹Specimens of the same type were also tested by an alternative *N. Gonorrhoeae* NAAT assay with the following results (# positive results / # samples tested): ^a0/1; ^b0/1; ^c0/1; ^d1/1.

²Specimens of the same type were also tested by an alternative *N. Gonorrhoeae* NAAT assay with the following results (# negative results / # samples tested): ^a0/1; ^b0/1; ^c1/3; ^d1/2.

³Score CI.

⁴PPV 95% CI computed from the exact 95% CI for the positive likelihood ratio, NPV 95% CI computed from the exact 95% CI for the negative likelihood ratio.

Table 12 shows the sensitivity, specificity, PPV, and NPV of the Aptima GC assay on the Panther system and the prevalence of *N. gonorrhoeae* (based on the specimen-specific PIS) in each specimen type by collection site. Prevalence varied across collection sites, as expected.

Table 12: Performance Characteristics of the Aptima Neisseria gonorrhoeae Assay by Collection Site

Specimen Type	Site	N	TP	FP	TN	FN	Prev %	Sensitivity % (95% CI) ¹	Specificity % (95% CI) ¹	PPV % (95% CI) ²	NPV % (95% CI) ²
PVS	1	21	3	0	18	0	14.3	100 (43.9, 100)	100 (82.4, 100)	100 (46.2, 100)	100 (89.5, 100)
	2	383	5	0	378	0	1.3	100 (56.6, 100)	100 (99.0, 100)	100 (57.7, 100)	100 (99.3, 100)
	3	75	0	0	75	0	0.0	NC	100 (95.1, 100)	NC	100 (NC)
	4	5	0	0	5	0	0.0	NC	100 (56.6, 100)	NC	100 (NC)
	5	254	5	0	249	0	2.0	100 (56.6, 100)	100 (98.5, 100)	100 (57.7, 100)	100 (99.0, 100)
	6	494	9	1	483	1	2.0	90.0 (59.6, 98.2)	99.8 (98.8, 100)	90.0 (63.1, 99.6)	99.8 (99.1, 100)
	7	246	4	1	241	0	1.6	100 (51.0, 100)	99.6 (97.7, 99.9)	80.0 (39.9, 99.4)	100 (99.0, 100)
	8	95	0	0	95	0	0.0	NC	100 (96.1, 100)	NC	100 (NC)
	9	313	1	0	312	0	0.3	100 (20.7, 100)	100 (98.8, 100)	100 (6.4, 100)	100 (99.7, 100)
	10	255	11	0	243	1	4.7	91.7 (64.6, 98.5)	100 (98.4, 100)	100 (76.3, 100)	99.6 (98.1, 100)
	11	96	0	0	96	0	0.0	NC	100 (96.2, 100)	NC	100 (NC)

Table 12: Performance Characteristics of the Aptima Neisseria gonorrhoeae Assay by Collection Site

Specimen Type	Site	N	TP	FP	TN	FN	Prev %	Sensitivity % (95% CI) ¹	Specificity % (95% CI) ¹	PPV % (95% CI) ²	NPV % (95% CI) ²
FU	1	22	3	0	19	0	13.6	100 (43.9, 100)	100 (83.2, 100)	100 (46.1, 100)	100 (90.0, 100)
	2	385	5	0	379	1	1.6	83.3 (43.6, 97.0)	100 (99.0, 100)	100 (59.6, 100)	99.7 (99.0, 100)
	3	74	0	0	74	0	0.0	NC	100 (95.1, 100)	NC	100 (NC)
	4	5	0	0	5	0	0.0	NC	100 (56.6, 100)	NC	100 (NC)
	5	250	5	0	245	0	2.0	100 (56.6, 100)	100 (98.5, 100)	100 (57.7, 100)	100 (98.9, 100)
	6	484	9	1	473	1	2.1	90.0 (59.6, 98.2)	99.8 (98.8, 100)	90.0 (63.1, 99.6)	99.8 (99.1, 100)
	7	245	4	0	241	0	1.6	100 (51.0, 100)	100 (98.4, 100)	100 (52.2, 100)	100 (99.0, 100)
	8	97	0	0	97	0	0.0	NC	100 (96.2, 100)	NC	100 (NC)
	9	261	0	0	261	0	0.0	NC	100 (98.5, 100)	NC	100 (NC)
	10	253	10	0	242	1	4.3	90.9 (62.3, 98.4)	100 (98.4, 100)	100 (74.6, 100)	99.6 (98.2, 100)
	11	91	0	0	91	0	0.0	NC	100 (95.9, 100)	NC	100 (NC)
MU	1	175	38	0	137	0	21.7	100 (90.8, 100)	100 (97.3, 100)	100 (91.3, 100)	100 (97.5, 100)
	2	373	3	0	370	0	0.8	100 (43.9, 100)	100 (99.0, 100)	100 (44.4, 100)	100 (99.4, 100)
	3	61	0	0	61	0	0.0	NC	100 (94.1, 100)	NC	100 (NC)
	4	13	0	0	13	0	0.0	NC	100 (77.2, 100)	NC	100 (NC)
	5	409	34	0	374	1	8.6	97.1 (85.5, 99.5)	100 (99.0, 100)	100 (90.5, 100)	99.7 (98.6, 100)
	6	307	28	1	278	0	9.1	100 (87.9, 100)	99.6 (98.0, 99.9)	96.6 (83.5, 99.9)	100 (98.8, 100)
	7	225	12	0	213	0	5.3	100 (75.8, 100)	100 (98.2, 100)	100 (76.6, 100)	100 (98.6, 100)
	8	32	0	0	32	0	0.0	NC	100 (89.3, 100)	NC	100 (NC)
	9	218	0	0	218	0	0.0	NC	100 (98.3, 100)	NC	100 (NC)
	10	91	10	0	80	1	12.1	90.9 (62.3, 98.4)	100 (95.4, 100)	100 (74.9, 100)	98.8 (94.6, 100)
	11	54	0	0	54	0	0.0	NC	100 (93.4, 100)	NC	100 (NC)

TP = true positive; FP = false positive; TN = true negative; FN = false negative; Prev = prevalence; CI = confidence interval; PPV = positive predictive value; NPV = negative predictive value; PVS = patient-collected vaginal swab; FU = female urine; MU = male urine; NC = not calculable.

¹ Score CI.

² PPV 95% CI computed from the exact 95% CI for the positive likelihood ratio, NPV 95% CI computed from the exact 95% CI for the negative likelihood ratio.

Neisseria gonorrhoeae Infected Status Tables

The frequency of test outcomes from reference NAAT and investigational Panther system testing is summarized in Table 13a and Table 13b.

Table 13a: *N. gonorrhoeae* Infected Status for Female and Male Urine Specimens

Specimen Type	Patient Infected Status	NAAT 1	NAAT 2	NAAT 3	AGC Assay	Symptom Status	
						Sym	Asym
FU	Infected	+	+	N/A	+	21	10
	Infected	+	+	N/A	-	0	2
	Infected	+	NR	+	+	1	0
	Infected	-	+	+	+	2	0
	Infected	-	+	+	-	0	1
	Infected	NR	+	+	+	1	1
	Non-infected	-	+	-	-	0	2
	Non-infected	-	-	N/A	+	0	1
	Non-infected	-	-	N/A	-	981	1077
	Non-infected	-	NR	-	-	1	1
MU	Infected	+	+	N/A	+	97	19
	Infected	+	+	N/A	-	2	0
	Infected	+	NR	+	+	1	0
	Infected	-	+	+	+	2	1
	Infected	NR	+	+	+	5	0
	Non-infected	+	-	-	+	1	0
	Non-infected	-	+	-	-	1	2
	Non-infected	-	-	N/A	-	689	1079
	Non-infected	-	-	N/A	=	0	1
	Non-infected	-	NR	-	-	1	0
Non-infected	NR	-	-	-	26	32	

Sym = symptomatic; **Asym** = asymptomatic; **AGC Assay** = Aptima Neisseria gonorrhoeae Assay; **FU** = female urine; **MU** = male urine; **N/A** = not applicable; **NR** = no result.

Note: The equal symbol (=) represents a final equivocal result.

Table 13b: *N. gonorrhoeae* Infected Status for Patient-collected Vaginal Swab Specimens

Patient Infected Status	NAAT 1		NAAT 2		AGC Assay	Symptom Status	
	PVS	FU	PVS	FU		Sym	Asym
Infected	+	+	+	+	+	20	12
Infected	+	+	+	+	-	0	1
Infected	+	+	+	NR	+	1	0
Infected	+	-	+	+	+	1	0
Infected	+	-	+	+	=	0	1
Infected	+	-	+	-	+	1	1
Infected	+	-	+	-	-	1	0
Infected	+	NR	+	+	+	0	1

Table 13b: *N. gonorrhoeae* Infected Status for Patient-collected Vaginal Swab Specimens

Patient Infected Status	NAAT 1		NAAT 2		AGC Assay	Symptom Status	
	PVS	FU	PVS	FU		Sym	Asym
Infected	-	+	+	+	+	1	0
Non-infected	+	-	-	-	-	2	0
Non-infected	-	-	+	+	+	1	0
Non-infected	-	-	+	-	-	2	2
Non-infected	-	-	-	+	-	0	2
Non-infected	-	-	-	-	+	0	1
Non-infected	-	-	-	-	-	961	1064
Non-infected	-	-	-	-	=	1	1
Non-infected	-	-	-	NR	-	1	0
Non-infected	-	-	NR	-	-	12	10
Non-infected	-	-	NR	NR	-	0	1
Non-infected	-	NR	-	-	-	37	25
Non-infected	NR	-	-	-	-	3	6
Non-infected	NR	NR	-	-	-	42	25

Sym = symptomatic; **Asym** = asymptomatic; **AGC Assay** = Aptima Neisseria gonorrhoeae Assay; **PVS** = patient-collected vaginal swab; **FU** = female urine; **NR** = no result.

Note: The equal symbol (=) represents a final equivocal result.

RLU Distribution of Aptima GC Assay Controls

The distribution of the RLU values for the Aptima GC assay controls is presented in Table 14 from all valid Panther system runs performed during the clinical study that included patient-collected vaginal swabs, and female and male urine specimens.

Table 14: RLU Distribution of Aptima GC Assay Negative and Positive Controls

Control	Statistic	Total RLU (x1000)
Positive Control, GC / Negative Control, CT	N	161
	Minimum	2416
	Median	5543.0
	Maximum	6477
	CV%	14.62
Positive Control, CT / Negative Control, GC	N	161
	Minimum	2
	Median	4.0
	Maximum	40
	CV%	93.85

CV% = percent coefficient of variation; **RLU** = relative light unit.

Note: The RLU value reported by the software was the basis for analysis. The reported RLU value is the total measured RLU divided by 1000 with the digits after the decimal point truncated.

Analytical Performance

Analytical Sensitivity (DTS)

N. gonorrhoeae analytical sensitivity (limit of detection) was determined by directly comparing dilutions of 51 different clinical isolates in culture and in the Aptima GC assay. The analytical sensitivity claim for the assay is 50 CFU/assay (362 CFU/swab, 250 CFU/mL urine, and 487.5 CFU/mL PreservCyt solution Pap).

Analytical Sensitivity Equivalence Study (Tigris)

Sensitivity panels in endocervical swab pool, vaginal specimen pool, urine specimen pool, and PreservCyt solution Pap specimen pool were prepared at GC 250 fg/assay rRNA and tested 60 replicates on the Tigris DTS system. Percent positivity (95% CI) on the Tigris DTS system for endocervical swab specimen was 100% (95.1–100), for vaginal swab specimen was 100% (95.1–100), for urine specimen was 100% (95.1–100), and PreservCyt solution Pap specimen was 100% (95.1–100).

GC rRNA Spiked Clinical Panel Study (DTS and Tigris)

The GC rRNA spiked clinical panel study evaluated agreement between the two systems using six Hologic prepared GC clinical panels spiked with 0 to 250,000 fg rRNA/assay of GC. The GC clinical panels were created from endocervical swab, vaginal swab, urethral swab, male urine, female urine, and PreservCyt solution Pap specimens that had negative Aptima GC results on the DTS systems when tested at Hologic. The negative specimens were pooled by specimen type, spiked or not spiked with GC rRNA and aliquotted as replicates of each panel member. Replicates of each of 6-panel members with different spiked rRNA levels were combined to create one clinical panel for each specimen type. Each panel contained a total of 132 replicates.

The initial male and female urine data show that some panel members that contained rRNA at a level below the claimed analytical sensitivity yielded unexpected negative results on the Tigris DTS system. Two follow-up studies were conducted to demonstrate and confirm agreement to expected results in spiked male or female urine panels. The original study design combined negative samples into a single master pool. The follow-up study design for male and female urine specimens was amended. The specimens were aliquotted into confirmed negative mini-pools to make the positive and negative panels. One hundred thirty-eight replicates were created for each panel.

Table 15 shows the percent agreement for each level of rRNA in the endocervical swab, vaginal swab, urethral swab, male urine, female urine, and PreservCyt solution Pap panels, respectively, with expected GC results for the Tigris DTS system and for the DTS systems. The concentration ranged from 1 log below to 3 logs above the 250 fg rRNA/assay for GC. Also shown in Table 15 are the overall percent agreements of the clinical panel study between the Tigris DTS system and DTS systems.

Table 15: GC rRNA Spiked Clinical Panel Agreement Study

Specimen	Panel Member	Concentration (fg rRNA/Assay)	Replicates	Tigris % Agreement	DTS % Agreement	Overall % Agreement between Tigris and DTS (95% CI)
Endocervical	No Target	0	12	100	100	100 (97.2–100)
	Very Low	25	30	100	100	
	Low	250	30	100	100	
	Medium	2,500	30	100	100	
	High	250,000	30	100	100	
Swab	No Target	0	12	100	100	100 (97.2–100)
	Very Low	25	29*	100	100	
	Low	250	30	100	100	
	Medium	2,500	30	100	100	
	High	250,000	30	100	100	
Urethral	No Target	0	12	100	100	100 (97.2–100)
	Very Low	25	30	100	100	
	Low	250	30	100	100	
	Medium	2,500	30	100	100	
	High	250,000	30	100	100	
Initial Study	No Target	0	12	100	100	91.7 (85.6–95.8)
	Very Low	25	30	63.3 (19/30)	100	
	Low	250	30	100	100	
	Medium	2,500	30	100	100	
	High	250,000	30	100	100	
Male Urine	No Target	0	18	100	100	100 (97.4–100)
	Very Low	25	30	100	100	
	Low	250	30	100	100	
	Medium	2,500	30	100	100	
	High	250,000	30	100	100	
Follow-up 2	No Target	0	18	100	100	100 (97.4–100)
	Very Low	25	30	100	100	
	Low	250	30	100	100	
	Medium	2,500	30	100	100	
	High	250,000	30	100	100	

*Not tested on both systems due to insufficient sample volume

Table 15: GC rRNA Spiked Clinical Panel Agreement Study (continued)

Specimen	Panel Member	Concentration (fg rRNA/Assay)	Replicates	Tigris % Agreement	DTS % Agreement	Overall % Agreement between Tigris and DTS (95% CI)
Initial Study	No Target	0	12	100	100	75.8 (67.5–82.8)
	Very Low	25	30	13.3 (4/30)	100	
	Low	250	30	80 (24/30)	100	
	Medium	2,500	30	100	100	
	High	250,000	30	100	100	
Female Urine	No Target	0	18	100	100	99.3 (96.0–100)
	Very Low	25	30	96.7 (29/30)	100	
	Low	250	30	100	100	
	Medium	2,500	30	100	100	
	High	250,000	30	100	100	
Follow-up 2	No Target	0	18	100	100	97.8 (93.8–99.5)
	Very Low	25	30	90 (27/30)	100	
	Low	250	30	100	100	
	Medium	2,500	30	100	100	
	High	250,000	30	100	100	
PreservCyt Solution Pap	No Target	0	12	100	100	100 (97.–100)
	Very Low	25	30	100	100	
	Low	250	30	100	100	
	Medium	2,500	30	100	100	
	High	250,000	30	100	100	

*Not tested on both systems due to insufficient sample volume

Spiked Clinical Panel Agreement Study (Tigris and Panther)

Individual negative urine specimens were spiked with GC to create a panel of 120 GC positives. GC positive panel members were spiked with organisms at 12.5 CFU/mL, 125 CFU/mL, or 1250 CFU/mL (25 fg/assay, 250 fg/assay or 2500 fg/assay). In addition, 120 GC negative urine specimens were collected. The positive and negative panels were tested on three Panther and three Tigris DTS systems. Positive percent agreement between the Panther system and the Tigris DTS system was 100% with a lower 95% confidence interval of 98.9. Negative percent agreement between the Panther system and the Tigris DTS system was 100% with a lower 95% confidence interval of 98.9. The results of the study are shown in Table 16.

Table 16: Spiked Clinical Panel Agreement Study: Agreement with Expected GC Results

Panel Member	Concentration		Replicates	Tigris % Agreement	Panther % Agreement
	CFU/mL	fg/assay			
Very Low Positive	12.5	25	117	100	100
Low Positive	125	250	120	100	100
Medium Positive	1,250	2500	120	100	100
Negative	0	0	360	100	100

Overall Positive Percent Agreement between Tigris DTS and Panther (95% CI): 100% (98.9–100).

Overall Negative Percent Agreement between Tigris DTS and Panther (95% CI): 100% (98.9–100).

Analytical Sensitivity Study (Panther)

Analytical sensitivity of the Aptima GC assay was tested using three representative specimen types. These were urine, PreservCyt solution Pap specimens, vaginal swabs, and STM (as control). GC rRNA was spiked into pools of these three specimen matrices at the following concentrations: 25 fg/assay and 250 fg/assay (rRNA equivalents of 12.5 CFU/mL and 125 CFU/mL). The rRNA equivalents were calculated based on the genome size and estimated DNA: RNA ratio/cell of each organism. These panels were tested on three Panther instruments using two lots of reagents in replicates of 60. Positive agreement with the expected result was calculated. Agreement to expected results was 100% (95% CI 95.7–100%) for all urine panels, 100% (95% CI 95.7–100%) for all PreservCyt solution Pap specimen panels, 100% (95% CI 95.7–100%) for all vaginal swab panels, and 100% (95% CI 96.1–100%) for all STM panels. The analytical sensitivity for the assay is 125 CFU/mL.

Analytical Specificity

A total of 154 culture isolates were evaluated using the Aptima GC assay. These isolates included 86 organisms that may be isolated from the urogenital tract and 68 additional organisms that represent a phylogenetic cross-section of organisms. The tested organisms included bacteria, fungi, yeast, parasites and viruses. All organisms except *C. psittaci*, *C. pneumoniae*, *U. urealyticum* and the viruses were tested at 1.0×10^6 cells/assay in KOVA-Trol Urine Transport Media (UTM) and 60 organisms were tested in STM. The Chlamydia and Neisseria organisms were tested in the PreservCyt solution media. *C. psittaci* (VR601) was tested at 8.0×10^4 cells/assay and *C. psittaci* VR125 was tested at 1.0×10^5 cells/assay. *C. pneumoniae* was tested at 4.0×10^3 cells/assay and *U. urealyticum* was tested at 6.7×10^6 cells/assay. The viruses were tested as follows: (a) herpes simplex virus I: 2.5×10^4 TCID₅₀/assay, (b) herpes simplex virus II: 6.0×10^4 TCID₅₀/assay, (c) human papillomavirus 16: 2.9×10^6 DNA copies/assay and (d) cytomegalovirus: 4.8×10^5 cells/assay. The list of organisms tested is shown in Table 17.

Table 17: Analytical Specificity

Organism	Organism	Organism
<i>Achromobacter xerosis</i>	<i>Escherichia coli</i>	<i>Neisseria mucosa</i> (3)
<i>Acinetobacter calcoaceticus</i>	<i>Flavobacterium meningosepticum</i>	<i>Neisseria sicca</i> (3)
<i>Acinetobacter lwoffii</i>	<i>Fusobacterium nucleatum</i>	<i>Neisseria subflava</i> (14)
<i>Actinomyces israelii</i>	<i>Gardnerella vaginalis</i>	<i>Neisseria perflava</i>
<i>Actinomyces pyogenes</i>	<i>Gemella haemolysans</i>	<i>Neisseria polysaccharea</i>
<i>Aerococcus viridans</i>	<i>Haemophilus ducreyi</i>	<i>Paracoccus denitrificans</i>
<i>Aeromonas hydrophila</i>	<i>Haemophilus influenzae</i>	<i>Peptostreptococcus anaerobius</i>
<i>Agrobacterium radiobacter</i>	Herpes simplex virus I	<i>Peptostreptococcus productus</i>
<i>Alcaligenes faecalis</i>	Herpes simplex virus II	<i>Plesiomonas shigelloides</i>
<i>Bacillus subtilis</i>	Human papillomavirus 16	<i>Propionibacterium acnes</i>
<i>Bacteriodes fragilis</i>	<i>Kingella dentrificans</i>	<i>Proteus mirabilis</i>
<i>Bacteriodes ureolyticus</i>	<i>Kingella kingae</i>	<i>Proteus vulgaris</i>
<i>Bifidobacterium adolescentis</i>	<i>Klebsiella oxytoca</i>	<i>Providencia stuartii</i>
<i>Bifidobacterium brevis</i>	<i>Klebsiella pneumoniae</i>	<i>Pseudomonas aeruginosa</i>
<i>Branhamella catarrhalis</i>	<i>Lactobacillus acidophilus</i>	<i>Pseudomonas fluorescens</i>
<i>Brevibacterium linens</i>	<i>Lactobacillus brevis</i>	<i>Pseudomonas putida</i>
<i>Campylobacter jejuni</i>	<i>Lactobacillus jensonii</i>	<i>Rahnella aquatilis</i>
<i>Candida albicans</i>	<i>Lactobacillus lactis</i>	<i>Rhodospirillum rubrum</i>
<i>Candida glabrata</i>	<i>Legionella pneumophila</i> (2)	<i>Saccharomyces cerevisiae</i>
<i>Candida parapsilosis</i>	<i>Leuconostoc paramensenteroides</i>	<i>Salmonella minnesota</i>
<i>Candida tropicalis</i>	<i>Listeria monocytogenes</i>	<i>Salmonella typhimurium</i>
<i>Chlamydia pneumoniae</i>	<i>Micrococcus luteus</i>	<i>Serratia marcescens</i>
<i>Chlamydia psittaci</i> (2)	<i>Moraxella lacunata</i>	<i>Staphylococcus saprophyticus</i>
<i>Chromobacterium violaceum</i>	<i>Moraxella osloensis</i>	<i>Staphylococcus aureus</i>
<i>Citrobacter freundii</i>	<i>Morganella morganii</i>	<i>Staphylococcus epidermidis</i>
<i>Clostridium perfringens</i>	<i>Mycobacterium smegmatis</i>	<i>Streptococcus agalactiae</i>
<i>Corynebacterium genitalium</i>	<i>Mycoplasma genitalium</i>	<i>Streptococcus bovis</i>
<i>Corynebacterium xerosis</i>	<i>Mycoplasma hominis</i>	<i>Streptococcus mitis</i>
<i>Cryptococcus neoformans</i>	<i>N. meningitidis</i> Serogroup A	<i>Streptococcus mutans</i>
Cytomegalovirus	<i>N. meningitidis</i> Serogroup B	<i>Streptococcus pneumoniae</i>
<i>Deinococcus radiodurans</i>	<i>N. meningitidis</i> Serogroup C (4)	<i>Streptococcus pyogenes</i>
<i>Derxia gummosa</i>	<i>N. meningitidis</i> Serogroup D	<i>Streptococcus salivarius</i>
<i>Eikenella corrodens</i>	<i>N. meningitidis</i> Serogroup Y	<i>Streptococcus sanguis</i>
<i>Enterobacter aerogenes</i>	<i>N. meningitidis</i> Serogroup W135	<i>Streptomyces griseinus</i>
<i>Enterobacter cloacae</i>	<i>Neisseria cinerea</i> (4)	<i>Trichomonas vaginalis</i>
<i>Enterococcus avium</i>	<i>Neisseria dentrificans</i>	<i>Ureaplasma urealyticum</i>
<i>Enterococcus faecalis</i>	<i>Neisseria elongata</i> (3)	<i>Vibrio parahaemolyticus</i>
<i>Enterococcus faecium</i>	<i>Neisseria flava</i>	<i>Yersinia enterocolitica</i>
<i>Erwinia herbicola</i>	<i>Neisseria flavescens</i> (2)	
<i>Erysipelothrix rhusiopathiae</i>	<i>Neisseria lactamica</i> (9)	

(n) = number of strains tested.

All organisms tested produced a negative result in the Aptima GC assay.

Analytical Specificity Equivalence Study

For a nucleic acid amplification assay, analytical specificity with respect to individual organisms is largely determined by the chemistry of the assay (e.g. oligonucleotide

sequences) rather than by the platform. Because the reagents for the Aptima GC assay are identical between the Panther system, Tigris DTS system and the DTS systems, analytical specificity experiments on the Panther system were designed to focus on the most challenging culture isolates. These organisms included those known to cross-react in other amplification assays. Twenty-five (25) culture isolates were selected from the panel of organisms in Table 17, including 17 organisms that are most closely related to GC. All of the organisms tested produced negative results.

Interfering Substances

The following interfering substances were individually spiked into swab, PreservCyt solution Pap, and/or urine specimens: 10% blood, contraceptive jelly, spermicide, moisturizer, hemorrhoidal anesthetic, body oil, powder, anti-fungal cream, vaginal lubricants, feminine spray and leukocytes (1.0×10^6 cells/mL). The following interfering substances were individually spiked into urine specimens: 30% blood, urine analytes, protein, glucose, ketones, bilirubin, nitrate, urobilinogen, pH 4 (acidic), pH 9 (alkaline), leukocytes (1.0×10^6 cells/mL), cellular debris, vitamins, minerals, acetaminophen, aspirin and ibuprofen. All were tested for potential assay interference in the absence and presence of GC at the estimated rRNA equivalent of 50 GC cells/assay (250 fg/assay). The rRNA equivalents were calculated based on the genome size and estimated DNA:RNA ratio/cell of each organism.

No interference was observed with any of the tested substances. No inhibitors of amplification were observed in the Aptima GC assay.

Interfering Substances Equivalence Study

Blood commonly found in urogenital specimens may interfere in some amplification assays. Whole blood was used to establish the degree of blood interference on the Panther system with respect to this potential interferant. Fresh blood was added to clinical pools of vaginal swab specimens, post-processed PreservCyt solution Pap specimens or urine specimens and then tested for potential assay interference in the presence and absence of GC target. The estimated rRNA equivalent of 125 GC CFU/mL (250 fg/assay) was used as the target concentration as this represents the analytical sensitivity of the assay. Specimens were tested on the Panther system. All samples containing target nucleic acid were positive when tested at a level of 10% (vol/vol) blood in swab or PreservCyt solution Pap specimens, or 30% (vol/vol) blood in urine specimens. All samples that did not contain target were correctly identified as negative. Blood added to swab, PreservCyt solution, and urine specimens at levels much higher than could be expected with normal specimen collection did not interfere with results on the Panther system.

Recovery

Escherichia coli, *Gardnerella vaginalis*, *Lactobacillus acidophilus*, *Bacteroides fragilis*, and *Staphylococcus epidermidis* (1.0×10^6 cells/assay) were added to samples containing the rRNA equivalent of approximately 50 GC cells (250 fg). These additions did not interfere with the amplification and detection of GC rRNA using the Aptima GC assay.

Specimen Stability Studies

A. Swab Specimens

Data to support the recommended shipping and storage conditions for endocervical, urethral and vaginal swab samples were generated with pooled negative swab samples. Pooled samples were spiked with GC at a final concentration of

approximately 50 CFU per reaction. The spiked samples were held at 4°C and 30°C. Samples were tested in duplicate at days 0, 20, 77, and 117. All test conditions were positive for GC at all times and temperatures.

B. Urine Specimens

Data to support the recommended shipping and storage conditions for urine samples were generated with female and male negative urine samples. The urine samples were spiked with GC at a final concentration of 100 CFU per reaction. The samples were held at 30°C for 24 hours prior to being added to the UTM. The UTM samples then were held at 4°C and 30°C and tested in triplicate at days 1, 14, 32 and 35. All replicates were positive for GC with UTM samples held at 4°C and 30°C.

C. PreservCyt Solution Pap Specimens

Data to support the recommended shipping and storage conditions for PreservCyt solution Pap samples were generated with negative processed and unprocessed liquid Pap samples. For the unprocessed samples, four pools of PreservCyt solution samples were tested after being stored in the PreservCyt solution vial. Each specimen pool was spiked with 50-100 CFU GC/assay, held at 2°C, 10°C, and 30°C, then tested at baseline and on days 5, 7, 8, 14, 18, 21, 25 and 36. All of the spiked samples were positive for GC at all times and temperatures.

For the processed samples, four pools of PreservCyt solution samples were used to determine processed specimen stability at 2°C to 30°C. Each negative sample pool was spiked with 50–100 CFU GC/assay, then tested at baseline. Prior to processing, the PreservCyt solution samples were stored at 30°C for seven (7) days to simulate the time-lapse between sample collection, Pap processing and shipment to a microbiology testing lab. After seven days at 30°C, 1 mL aliquots of each pool were transferred to an Aptima specimen transfer tube and tested at baseline before being placed at 2°C, 10°C, and 30°C. The processed samples were then tested for 17 days stored at 30°C and 36 days stored at 2°C to 10°C. All of the spiked samples were positive for GC at all times and temperatures.

D. Additional Frozen (at –20°C) Specimen Stability Study

The recommended frozen storage conditions for endocervical swab, urethral swab, vaginal swab, female urine, male urine, and PreservCyt solution Pap specimens in transport media is between –20°C to –70°C to allow testing up to 12 months after collection. Supporting data for each specimen type were generated using 90 negative specimens. Of these, 30 specimens were spiked with GC at 50 CFU per reaction; 30 specimens were spiked at 5 CFU per reaction; and 30 specimens were not spiked. The specimens in transport media were stored frozen within 7 days of collection and tested at days 200 and 400. Specimens met the acceptance criteria of 95% agreement with expected results.

Precision/Reproducibility Study

The Aptima GC assay precision was evaluated across three Panther systems, two Aptima GC assay kit lots, over a period of 24 days. Panels were made by spiking GC rRNA into STM at the concentrations shown in Table 18. Operators performed two runs per day running each panel member in replicates of two per run. The agreement with the expected result was calculated and precision was estimated according to NCCLS Guidelines EP5-A2 (11). The total number of replicates for each panel was 96. Table 18 presents the precision RLU data in terms of Mean, Standard Deviation, Coefficient of Variation (CV), percent agreement with expected results and calculations of between-instrument, between-lot, between-run, and within-run variability.

Table 18: Panther Precision for Aptima GC Assay

Matrix	GC (CFU/mL)	N	Mean RLU (x1000)	% Agrmt	Between-instrument		Between-lot		Between-Run		Within-Run		Total	
					SD (x1000)	CV (%)	SD (x1000)	CV (%)	SD (x1000)	CV (%)	SD (x1000)	CV (%)	SD (x1000)	CV (%)
STM	0	96	3	100	0	0	0	0	0	0	2.01	72.8	2	72.5
	12.5	96	3951	100	215.14	5.4	0	0	0	0	568.24	14.4	607.6	15.4
	125	95 ¹	5839	100	370.17	6.3	0	0	0	0	772.58	13.2	856.7	14.7
	1250	96	6207	100	338.25	5.4	0	0	0	0	787.64	12.7	857.2	13.8
Urine	0	95 ¹	3	100	0.69	21.6	0.81	25.5	0.77	24.2	2.43	76.3	2.8	87.8
	12.5	96	3460	100	0	0	195.84	5.7	113.27	3.3	207.53	6	307	8.9
	125	96	6047	100	158.67	2.6	170.32	2.8	0	0	206.24	3.4	311	5.1
	1250	96	6737	100	218.35	3.2	238.49	3.5	66.22	1	176.72	2.6	374.4	5.6
PreservCyt Solution	0	95 ¹	6	100	1.9	33.6	0	0	0.54	9.5	5.96	105.2	6.3	111.2
	12.5	96	3358	100	257.9	7.7	0	0	0	0	485.45	14.5	549.7	16.4
	125	96	5272	100	243.09	4.6	201.89	3.8	0	0	751.72	14.3	815.4	15.5
	1250	96	5945	100	355.95	6	51.06	0.9	0	0	759.35	12.8	840.2	14.1

SD = standard deviation; CV = coefficient of variation; RLU = relative light unit.

Note: Variability from some factors may be numerically negative, which can occur if the variability due to those factors is very small. When this occurs, SD = 0 and CV = 0%.

¹ The n of 95 indicates 1 invalid replicate out of 96 which was not repeated.

Carryover Studies for the Panther System

To establish that the Panther system minimizes the risk of false positive results arising from carryover contamination, a multi-run analytical study was conducted using spiked panels on three Panther systems. Carryover was assessed using approximately 20% high titer GC samples dispersed between negative samples. The runs included clusters of high positive samples with clusters of negative samples as well as single high positives dispersed in a specific pattern within the run. High titer samples were made using GC rRNA spiked into STM to give a final concentration of 5×10^5 fg rRNA/reaction (rRNA equivalent of 2.5×10^5 CFU/mL). Testing was carried out using 5 runs on three Panther systems with a total of 2923 negative samples. The overall carryover rate was 0% with a 95% confidence interval of 0–0.1%. A total of 17 negative samples from the high titer runs were reported as invalid and were excluded from the calculation.

Bibliography

1. **Centers for Disease Control and Prevention.** *Morbidity and Mortality Weekly Report*, 2021. Sexually Transmitted Infections Treatment Guidelines. 70(4), July 23, 2021.
2. **Holmes, K. K., H. H. Handsfield, S. P. Wang, B. B. Wentworth, M. Turck, J. B. Anderson, and E. R. Alexander.** 1975. Etiology of nongonococcal urethritis. *NEJM* 292:1199-1205.
3. **Masi, A. T., and B. I. Eisenstein.** 1981. Disseminated Gonococcal Infections (DGI) and Gonococcal Arthritis (GCA): II Clinical Manifestations, Diagnosis, Complications, Treatment and Prevention. *Semin. Arthritis Rheum.* **10**:173.
4. **Hook III, E. W. and H. H. Handsfield.** 1999. Gonococcal Infections in the Adult. p. 458. In K. Holmes et. al. (eds.) *Sexually Transmitted Diseases*. McGraw Hill, New York, N.Y.
5. **Ching, S., H. Lee, E. W. Hook, III, M. R. Jacobs, and J. Zenilman.** 1995. Ligase chain reaction for detection of *Neisseria gonorrhoeae* in urogenital swabs. *J. Clin. Microbiol.* 33:3111-3114.
6. **Krauss, S. J., R. C. Geller, G. H. Perkins, and D. L. Rhoden.** 1976. Interference of *Neisseria gonorrhoeae* growth by other bacterial species. *J. Clin. Microbiol.* 4:288-295.
7. **Farrel, D. J.** 1999. Evaluation of AMPLICOR *Neisseria gonorrhoeae* PCR using cppB nested PCR and 16S rRNA PCR. *J. Clin. Microbiol.* **37**:386-390.
8. **Chong, S., D. Jang, X. Song, J. Mahony, A. Petrick, P. Barriga, and M. Chernesky.** 2003. Specimen Processing and Concentration of *Chlamydia trachomatis* Added Can Influence False-Negative Rates in the LCx Assay but Not in the Aptima Combo2 Assay When Testing for Inhibitors. *J. Clin. Microbiol.* 41:778-782.
9. **Gaydos, C. A., T. C. Quinn, D. Willis, A. Weissfeld, E. W. Hook, D. H. Martin, D. V. Ferraro, and J. Schachter.** 2003. Performance of the Aptima Combo 2 Assay for Detection of *Chlamydia trachomatis* and *Neisseria gonorrhoeae* in Female Urine and Endocervical Swab Specimens. *J. Clin. Microbiol.* 41:304-309.
10. **Public Health England.** 2021. Guidance for the detection of gonorrhoea in England.
11. National Committee for Clinical Laboratory Standards. 2004. NCCLS EP5-A2: Evaluation of Precision Performance of Quantitative Measurement Methods: Approved Guideline (2nd edition, Vol. 24, No. 25).

Contact Information and Revision History



Hologic, Inc.
10210 Genetic Center Drive
San Diego, CA 92121 USA



Hologic BV
Da Vincilaan 5
1930 Zaventem
Belgium

Australian Sponsor
Hologic (Australia & New Zealand) Pty Ltd.
Macquarie Park NSW 2113

For country-specific Technical Support and Customer Service email address and telephone number, visit www.hologic.com/support.

Serious incidents occurring in relation to the device in the European Union should be reported to the manufacturer and the competent authority of the Member State in which the user and/or the patient is established.

Hologic, Aptima, Aptima Combo 2, DTS, Panther, Panther Fusion, PreservCyt, ThinPrep, Tigris, and TMA are trademarks and/or registered trademarks of Hologic, Inc. and/or its subsidiaries in the United States and/or other countries.

TECAN is a trademark of Tecan Group AG.

All other trademarks that may appear in this package insert are the property of their respective owners.

This product may be covered by one or more U.S. patents identified at www.hologic.com/patents.

© 2003–2024 Hologic, Inc. All rights reserved.

AW-31111-001_001 Rev. 001
2024-07

Revision History	Date	Description
AW-31111 Rev. 001	July 2024	<ul style="list-style-type: none"> Creation of an APTIMA GC IVDR-compliant assay IFU AW-31111 Rev. 001 for commercialization (ExUS) using APTIMA GC IVDR-compliant assay IFU AW-31111 Rev. 001, IVDR, Regulatory Submission (ExUS) as template Updated the SDS section according to the latest SDS revisions Performed administrative edits and updates throughout