

Table of Contents

1. INTRODUCTION 2

2. SYSTEM OVERVIEW 4

3. WARNINGS and CAUTIONS..... 6

4. USING THE SYSTEM 8

5. USING THE CONTROLS..... 11

6. IN SURGERY 13

7. AFTER SURGERY..... 16

8. SPECIFICATIONS..... 17

9. TROUBLESHOOTING 18

10.DISPOSAL..... 19

11.SYMBOLS 19

12.EMC DECLARATION 20

13.FCC INFORMATION..... 26

14.TECHNICAL SUPPORT AND PRODUCT COMPLAINTS..... 26

15.REPLACEMENT PARTS..... 27

16.REPLACING THE POWER SUPPLY INTERCHANGEABLE PLUG..... 28

1. INTRODUCTION

Please read all information carefully. Failure to properly follow the instructions may lead to unintended consequences.

Patient Target Group

The **TruNode** Gamma Probe system is intended to be used on patients presenting with a need to detect gamma radiation from Tc-99m and I-125 radionuclides in the body or tissues.

Intended User

The **TruNode** Gamma Probe is intended to be used by physicians.

Indications for Use

The **TruNode** Gamma Probe System can be used in non-imaging procedures to quantify relative amounts of Tc-99m or I-125 radionuclides in a particular organ or body region. It can be used in transcutaneous, open surgical, and laparoscopic procedures.

Device Description

The **TruNode** Gamma Probe System is designed to detect and quantify Technetium-99m (Tc-99m) and Iodine-125 (I-125) in radio-guided localization medical procedures. A numeric display and audible signal convey the relative amount of radiation detected, allowing the user to localize radiolabeled tissue or structures.

The system is battery-powered, wireless, and portable. It consists of the **TruNode** Gamma Probe and the **TruNode** User Feedback Unit.

Potential Applications

The **TruNode** Gamma Probe System can be used by physicians for radio-guided localization of tissues containing Technetium-99m (Tc-99m) and Iodine-125 (I-125). Potential applications include: radio-guided 'sentinel' lymph node localization with Tc-99m-labeled radiotracer, radio-guided parathyroidectomy with a Tc-99-labeled radiopharmaceutical such as Sestamibi, and radio-guided tumor localization with 'seeds' containing I-125 isotope.

Clinical Benefits

The **TruNode** Gamma Probe System is designed to assist physicians in locating radiolabeled tissue or structures impacting procedural success.

Adverse Effects

The following adverse effects could occur with the use of the **TruNode** Gamma Probe system:

- Reuse of the probe could result in cross-infection and cross-contamination
- Use of another power supply may increase the risk of electric shock

2. SYSTEM OVERVIEW

The **TruNode** User Feedback Unit is used with the **TruNode** Probe.

TruNode User Feedback Unit (UFU)

The UFU is comprised of an off-the-shelf tablet computer and custom speaker all enclosed in a custom protective silicone rubber case. An IV pole clamp is attached to the back. The tablet computer uses the Android operating system and runs the **TruNode** Application.



TruNode UFU

A medical-grade power supply is included for re-charging the UFU battery.



Low-leakage Medical Grade Power Supply

The UFU communicates bi-directionally with the TruNode Probe over a Bluetooth Low Energy ('BLE') wireless link. It provides the visual display, sound feedback, and redundant controls for operating the probe.

The rate of gamma photons entering the Probe is displayed on the UFU in digits and with a log-scale meter. This rate is also represented by the audio feedback (pitch and beat frequency) coming from the speaker. The UFU will also announce the count rate upon request by the user via pushbutton on the Probe handpiece.

The tablet computer controls for changing parameters such as the time zone or the announcements are accessed through the touch screen interface, as with any Android operating system. The ON/OFF control that turns ON the UFU and launches the **TruNode** application is located on the top of the UFU enclosure.

TruNode Probe

The wireless **TruNode** Probe is battery-powered (4.5V). It is completely sealed and supplied sterile for a single-patient use in a Tyvek™ peel-pouch. The pouch is designed for sterile handoff. The Probe can also be used in the pouch without breaking the seal prior to setting up the sterile field. Prior to use, the Probe must be stored in its unit box to prevent damage to the sterile pouch.

The Probe detects and quantifies gamma rays ('counts') from Tc-99m and I-125 isotopes and communicates this information to the UFU over the wireless link for user feedback. The Probe keypad provides the user with control of:

- activation status,
- detection energy window mode*,
- audio count-rate feedback volume,
- audio count-rate range scaling,
- announce instantaneous count-rate feedback, and
- announce integrated count-rate feedback*.

*see 'Using the Controls', Section 5.

3. WARNINGS and CAUTIONS

General

- Prior to use of the **TruNode** Probe, inspect the protective packaging and device to verify that neither has been damaged during shipment. If it appears the packaging has been compromised, do not use the device.
- Failure to thoroughly review and adhere to the information contained in this User Manual may pose a potential hazard to the patient and/or the user and may void the warranty.
- The **TruNode** Gamma Probe System is not intended for use in the central nervous system.
- Do not modify this equipment without the authorization of the manufacturer.

User Feedback Unit

- Use only the Hologic Power Supply provided with the UFU for recharging. The use of another power supply may increase the risk of electric shock.
- Fully charge the UFU before using the system.
- Do not use the Charger in the operating room.
- Do not use the Charger in the presence of an oxygen-enriched environment or in the presence of a flammable anesthetic mixture with air or with oxygen or nitrous oxide.
- Keep the UFU off when charging.
- Remove the Charger when the UFU is fully charged.
- The UFU and Charger are non-sterile. Do not sterilize these components.
- If liquid is spilled on the UFU, remove it from service and contact Hologic for instructions to return for inspection.
Ph: 1. 877.910.0030.
- Securely mount the UFU to an IV pole.
- After connecting to a probe, the UFU must be turned 'off' then back 'on' before attempting to connect to a new probe.

Probe

- DO NOT activate the Probe until it is ready to be used. It is designed to be used immediately after activation.
- Keep a spare Probe at the ready in case of a failure, or of exceeding its 95-100-minute life after activation, or of exceeding its 4-hour life window.
- DO NOT reuse the Probe. It can be used on a single patient in a single surgical procedure only. Reuse poses a risk of cross-infection and cross-contamination.
- DO NOT attempt to re-sterilize the Probe.
- DO NOT drop the Probe. It may damage the detector element.
- DO NOT strike the Probe tip against a hard surface. It may damage the detector element.
- DO NOT simultaneously use the probe together with an electro-surgery device. It can disrupt the detector and produce spurious counts.
- DO NOT touch the probe to an energized electro-surgery device. It can damage the probe.

4. USING THE SYSTEM

Setting the Language (As required for use outside the United States)

1. Turn on the UFU by pressing down on the ON-OFF control switch, located on its top-left edge, for approximately 5 seconds, or until the boot screen appears.
2. Allow the UFU to completely boot.
3. Close the TruNode application by touching the UFU screen to bring up the bottom menu and tap the icon that has 3 vertical lines (III), then touch **Close All**.
4. Open the settings window by touching the **Settings** icon  on the home page.
5. Scroll down to General Management and select it by touching the screen. Then select **Language and Input** followed by **Language**.
6. Drag the desired language to the top of the list and then touch **Apply**.
7. Turn the UFU OFF, then ON again, as described above, to verify the language is set correctly.

Setting up the UFU (to be done prior to starting the procedure)

1. Turn on the UFU by pressing down on the ON-OFF control switch located on its top-left edge for approximately 5 seconds, until the boot screen appears.


If only the battery-charge ICON  appears, the battery is fully depleted and the UFU must be recharged prior to use.

NOTE: *It takes about three hours to fully charge a fully discharged UFU.*

Unless the UFU is fully depleted, the Android 'Home' screen will appear after 40 seconds.


After another 30 seconds, the **TruNode** application will launch and the UFU will be ready to detect the **TruNode** probe.

***NOTE:** If the TruNode app icon is pressed before it opens automatically it will still launch OK, but the warning below may appear. If so, click OK.*

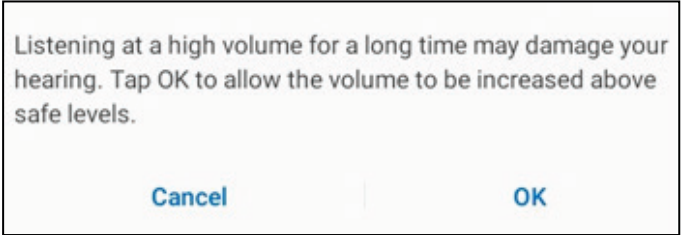

***Caution:** If the battery charge is below 50%, turn off the UFU and charge it prior to use. Do not use the Charger in the operating room.*


- 2. The UFU will announce a greeting followed by its charge status. Verify the UFU is at least 50% charged prior to starting the procedure.
- 3. When an image of the probe keypad with a flashing ‘M’ button is displayed, the UFU is ready to link with a **TruNode** Probe.
- 4. Clamp the UFU securely to an IV pole in a location that is easy to see by the user.

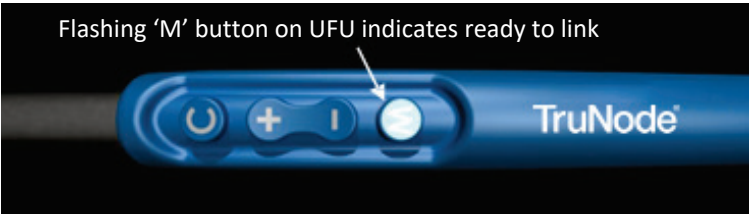

***NOTE:** After connecting to a probe, the UFU must be turned ‘off’ then back ‘on’ before attempting to connect to a new probe.*

Deploying the Probe

1. Remove the Probe from the sterile peel-pouch, using an aseptic technique.

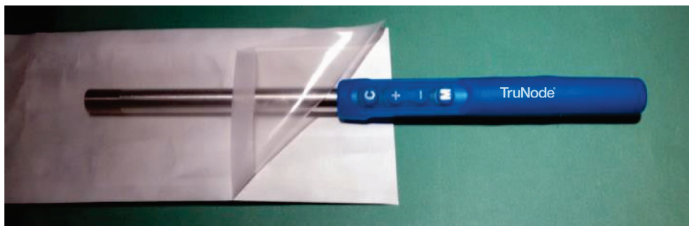

2. Activate the Probe by pressing and holding the 'M' button until the light on the Probe keypad flashes. This indicates the Probe has been activated. The live **TruNode** application will start when the UFU senses the Probe.



NOTE: The **TruNode** Probe can be used preoperatively in its sterile pouch prior to sterile deployment. Simply press through the clear *poly film* to access the controls. Use care not to damage the pouch seals, as this could disrupt its sterile barrier.

NOTE: The battery charge in the **TruNode** Probe can also be tested as in step 2 by first assuring there is no UFU in 'Ready' state nearby – a flashing light indicates the battery is not discharged. If no UFU is detected, the probe will turn off in 30 seconds.

NOTE: The useful life of the **TruNode** Probe is the lesser of 95-100 minutes of continuous use, one patient procedure, or 4 hours, including preoperative use.


NOTE: The **TruNode** Probe will hibernate after 10 minutes of inactivity. To awaken the probe, simply press and hold the 'M' button until the light on the keypad flashes.

NOTE: The UFU will display the life of the probe when 15 minutes of use or less remain.


5. USING THE CONTROLS

NOTE: Each button can be: 1) momentarily ‘clicked’ or 2) held down for ~2 seconds to initiate a function. The UFU will announce the function.

- To adjust the audio count-rate feedback volume:** Click the ‘+’ or ‘-’ button on the probe. A slider bar on the UFU displays the volume. The volume of the announcements cannot be adjusted.

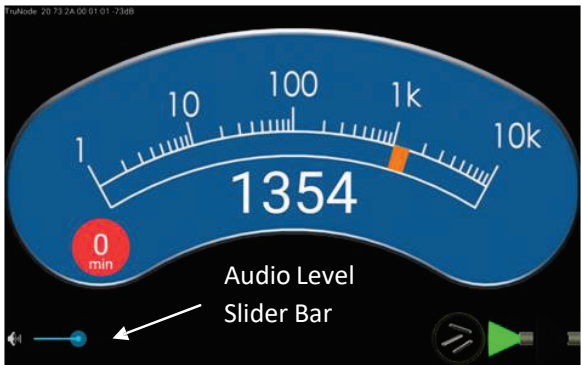

- To mute the audio feedback volume:** Repeatedly click the ‘-’ button on the Probe until the UFU announces “Muting Probe.” The audio level slider bar will be minimized, and the speaker icon will be displayed in red.
- To change the mode of the Probe from ‘Scan’ to ‘Point’:** Click the ‘M’ button on the Probe handle. The selected mode is displayed on UFU.
- To change the mode of the Probe to ‘Seed’ from ‘Scan’ or ‘Point’:** Hold the ‘M’ button down for 2 seconds. Seed mode is displayed on UFU.

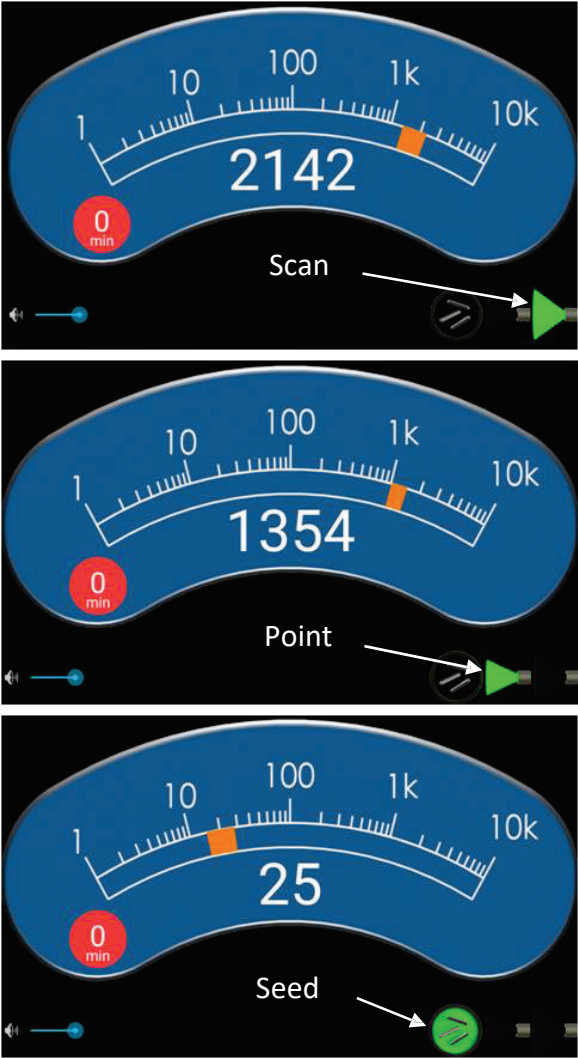

 **To announce the instantaneous count rate:** Click the 'C' button. The UFU continuously displays the instantaneous count rate.

-  **To get an averaged count rate:** Hold the 'C' button for 2 seconds - at which time "Recording Counts" will be announced – then a countdown to "Zero" while the integration completes – and finally the averaged count rate is announced and displayed on the UFU. Up to 6 of the most recent average count rates can be displayed, and they can be removed by touching the stored count rate on the display.
-  **To change the audio scale to match the count range:** Hold the '+' Button for 2 seconds – at which time "High Range" will be announced, and the audio feedback will reflect the higher range. Clicking the '-' button will toggle back to low Range.

6. IN SURGERY

CHANGING MODES

Three photon energy-resolving modes are available -- 'Scan' and 'Point' modes are used for detecting Tc-99m. 'Seed' mode is used for detecting I-125.

Scan mode provides higher sensitivity because it counts more gamma photons that have been scattered while in transit from their source to the probe's detector. This allows the user to survey wider areas more quickly than Point mode. The relatively higher number of gamma photons that are detected produce more rapid count-rate feedback information, and Scan mode accepts scattered gamma photons with lower energy than Point mode, and thus could have emanated from a wider region. Scan mode can be used for surveying larger areas, more quickly, especially when there is less background or scattered radiation (e.g., from the injection site or nearby organs that uptake radiotracer). Scan mode can also be used to obtain more accurate ex-vivo specimen count rates because of its wider angle of acceptance for scattered gamma photons that may be emanating from the specimen.

Point mode provides higher-spatial resolution because it rejects low-energy gamma photons that have been scattered while in transit from their source to the probe's detector.

This allows the user to more precisely locate the source of the gamma photons: only those photons that have been minimally scattered between their source and the probe's detector are counted, so the influence of background and scattered radiation is reduced. Point mode can be used when searching for hotspots where there is predominate background or scattered radiation (e.g., from the injection site or nearby organs that uptake radiotracer), and when attempting to more accurately localize small radioactive hotspots.

Seed mode preferentially accepts photons from I-125, while rejecting the majority of photons from nearby Tc-99m. This can be useful for detecting I-125 seeds or other sources of I- 125 isotope.

CHANGING THE AUDIO SCALE TO MATCH THE INCOMING COUNT RATE

A range of audio feedback is produced in proportion to the range of detected count rates. An increase in pitch and beat frequency indicates an increase in the detected count rate. Two audio ranges are used to cover the range of count rates detectable by the **TruNode** System. When the Probe is initialized, it defaults to the low range, producing audio feedback for count rates up to 2,000 counts per second. When more than 2,000 counts per second are detected, the very high-pitched sound alerts the user that the high range may be needed. High range detects photons up to 10,000 counts per second.

NOTE: *The selected range does not affect the digital count display or the count rate-meter.*

OBTAINING AN AVERAGED COUNT RATE

The user can initiate the acquisition of an averaged, statistically-significant count rate to improve the accuracy of the count rate reading for an exact target region. The user must hold the probe perfectly steady during this acquisition. When this feature is initiated, the **TruNode** System will:

For count rates greater than or equal to 40 counts per second.

The system will count for 2-10 seconds and return a count rate measurement with better than or equal to $\pm 10\%$ accuracy with 95% confidence. Very high-count rates will be measured very quickly to very high accuracy (e.g., 1,000CPS target: 2 seconds counting time, $\pm 10\%$ accuracy with 99% confidence).

Or

For count rates below 40 counts per second. The system will count for 10 seconds and return a count rate measurement that is more accurate than the instantaneous reading but to less than $\pm 10\%$ accuracy with 95% confidence. Very low count rates will have much lower accuracy (e.g., 5CPS target: 25% accuracy with 95% confidence).

7. AFTER SURGERY

- ✚ Dispose of the Probe in an appropriate bio-hazardous waste container.



Discard electrical and electronic equipment separately from standard waste. Send decommissioned material to Hologic or contact your service representative.

- ✚ Turn off the UFU:

- Press the ON-OFF control switch located on its top-left edge for approximately 2 seconds until the power off options appear.
- Follow the instructions that appear for powering off the UFU.

NOTE: *The UFU must be turned off before the next procedure or it will not connect with another Probe.*

- Wipe the surfaces of the UFU with a damp cloth or disinfectant wipe if they are soiled. Clean the display screen with a dry cloth to remove smudges.
- Charge the UFU. For maximum battery life, remove the charger when the UFU is fully charged.

8. SPECIFICATIONS

TruNode Probe

Overall Dimensions: 17mm X 226mm

Reach: 103mm, Operative Diameter: 10mm

Weight: 70g

Wireless: Bluetooth® Smart

Integrated Tungsten Collimator

External Materials: Stainless Steel, Tungsten, Silicone Rubber

Shielding Efficiency: >99.9%

Energy Resolution: 10% FWHM (Tc-99m)

Selectable Energy Windows:

Tc-99 'Point' Mode, Tc-99 'Scan' Mode, I-125 'Seed' Mode

Angular Resolution in Air: 46 degrees FWHM

Spatial Resolution @1cm in Air, Point Mode: 13mm FWHM

Spatial Resolution @1cm in Air, Scan Mode: 14mm FWHM

Sensitivity in Air, Point Mode: 18,000CPS/MBq max; 3,400 /MBq @1cm

Sensitivity in Air, Scan Mode: 27,000CPS/MBq max; 4,800CPS/MBq @1cm

Probe-Mounted Controls:

Activate & Connect to UFU

Mode (Hi-Sensitivity 'Scan', Hi-Resolution 'Point', I-125 'Seed'),

Count Rate Reporting,

Count Rate Averaging,

Audio Feedback Scaling,

Volume and Mute.

Probe Life: Lesser of 95-100-min continuous use, or 4-hr intermittent use, or 1-procedure

Use Condition Limitation: 15 to 37°C

Storage & Transit Condition Limitation: -15 to 50°C

TruNode User Feedback Unit

Overall Dimensions: 25cm x 18cm x 2.3/13cm (without/with clamp)

Weight 1.4kg (with clamp)

Android operating system, Maintenance free, no calibration

Power Supply: TRUMPower Medical Power Supply, P/N TMW15-5-IUB

Input 100-240VAC, 56/60Hz; Output 5VDC, 3A

Storage & Transit Condition Limitation: -15 to 50°C

9. TROUBLESHOOTING



Symptom: radiation count rate greater than zero even when no radiation present after contacting radioactive tissue

Resolution: decontaminate probe tip of radioactive material using sterile process



Symptom: spurious radiation counts in conjunction with energizing electrocautery device or other radio-frequency emitter

Resolution: move electrocautery device cable or other radio-frequency emitter away from probe



Symptom: spurious radiation counts not associated with radiation contamination or electrocautery device or other radio-frequency emitter

Resolution: replace probe



Symptom: insufficient or complete lack of radiation counts when locating the probe over a known source of high radioactivity

Resolution: replace probe



Symptom: new probe or probe that has not expired won't connect with a UFU.

Resolution: turn the UFU off then back on – the UFU must be turned off prior to connecting to a new probe.

10. DISPOSAL

-  Dispose of the Probe in an appropriate bio-hazardous waste container.
-  Follow local regulations for disposal of all other TruNode components when at the end of life.

11. SYMBOLS

R_X ONLY	Caution: Federal law restricts this device to sale by or on the order of a licensed healthcare practitioner	*
 IPX4	Splash-proof	*
	Type BF Applied Part	*
	Bluetooth®	*
	Use by date	*
 www.hologic.com/package-inserts	Consult instructions for use	* **
	Follow instructions for use	* **
	Sterilized using ethylene oxide	*
	Not to be used in case package is damaged	*
	Re-use is not allowed	*
	Do not re-sterilize	*
	Does not contain natural rubber latex	*
	Contains alkaline battery	*
	European Authorized Representative	**
	Manufacturer	* **
	Temperature limitation	* **
	Discard electrical and electronic equipment separately from standard waste. Send decommissioned material to Hologic or contact your service representative.	* **

	Serial number = Date of Manufacturer (YYMMDD-XX)	**
	Lot number	*
	Model	* * *
	Medical device	* * *
	Caution, consult documents	
	Single sterile barrier system with protective packaging outside	*
	Single sterile barrier system	**
	Compliant to AS/NZS 4268 for short range radio equipment, Australian Standard AS/NZS 4417.1, and AS/NZS 4417.2.	

*Affixed to Probe Label

**Affixed to UFU Label

12. EMC DECLARATION

This product has been tested and verified to ensure that there are no issues or concerns regarding reciprocal interference. This includes EMI, EMC, and RF. It has been certified and tested by 3rd party testing facilities. List of standards is as follows:

- Medical Electrical Equipment - Part 1: General Requirements For Safety - Collateral Standard: Electromagnetic Compatibility - Requirements and Tests – EN 60601-1-2:2014
- CFR 47, Part 15, Section 15.247 (b): Effective Isotropic Radiated Power (EIRP)
- CFR 47, Part 15, Section 15.247 (d): Spurious Emissions
- EMC Directive 2014/30/EU
- Radio Equipment Directive 1999/5/EC

The TruNode Gamma Probe System needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided in this User Manual. The customer or user of the TruNode Gamma Probe System should assure that it is used in such an environment. The following tables provide a guidance and declaration for the electromagnetic emissions and immunity of the TruNode Gamma Probe System which requires the use of the supplied TruNode Power Supply. The use of components other than these may result in increased emissions or

decreased immunity. Similarly, the use of the supplied Power Supply and Cable with equipment and systems other than the TruNode Gamma Probe System may significantly degrade emissions and immunity and result in improper operation.

Portable and mobile RF communications equipment can degrade the performance of the TruNode Gamma Probe System and should be used no closer than 30cm (12 inches) to any part of the system.

The TruNode Gamma Probe System should not be used adjacent to or stacked with other equipment. If adjacent or stacked use is necessary, the TruNode Gamma Probe System should be observed to verify normal operation in the configuration in which it will be used.

The TruNode Gamma Probe System transmitter and receiver use Bluetooth® SMART technology, with a frequency band of 2.400 GHz-2.4835 GHz and GFSK modulation. The effective radiated power of the transmitter is 1.2mW.

The TruNode Gamma Probe System may be interfered with by other equipment, even if that other equipment complies with CISPR EMISSION requirements.

Guidance and manufacturer’s declaration – electromagnetic emissions		
The TruNode Gamma Probe System is intended for use in the electromagnetic environment specified below. The customer or the user of the TruNode Gamma Probe System should assure that it is used in such an environment.		
Emissions Test	Compliance	
RF emissions CISPR 11	Group 1	The TruNode Gamma Probe System uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class A	The TruNode Gamma Probe System is suitable for use in all establishments other than domestic and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonic emissions IEC 61000-3-2	Class A	
Voltage Fluctuations/ Flicker emissions	Complies	

Guidance and manufacturer's declaration – electromagnetic immunity			
The TruNode Gamma Probe System is intended for use in the electromagnetic environment specified below. The customer or the user of the TruNode Gamma Probe System should assure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment – guidance
Electrostatic discharge (ESD) IEC 61000-4-2	±8 kV contact ±15 kV air	±8 kV contact ±15 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30 %.
Electrical fast transient/burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/output lines	±2 kV for power supply lines ±1 kV for input/output lines	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	±1 kV differential mode ±2 kV common mode	±1 kV differential mode ±2 kV common mode	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	Voltage Dips 30% reduction, 25/30 periods At 0°	Voltage Dips 30% reduction, 25/30 periods At 0°	Mains power quality should be that of a typical commercial or hospital environment. If the user of the TruNode Gamma Probe System requires continued operation during power mains interruptions, it is recommended that the TruNode Gamma Probe System be powered from an uninterruptible power supply or a battery.
	Voltage Dips > 95% reduction, 0.5 period At 0°, 45°, 90°, 135°, 180°, 225°, 270° and 315°	Voltage Dips > 95% reduction, 0.5 period At 0°, 45°, 90°, 135°, 180°, 225°, 270° and 315°	
	Voltage Dips > 95% reduction, 1 period At 0°	Voltage Dips > 95% reduction, 1 period At 0°	
	Voltage Interruptions > 95% reduction, 250/300 periods	Voltage Interruptions > 95% reduction, 250/300 periods	
(50/60 Hz) magnetic field IEC 61000-4-8	30 A/m	30 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.

Guidance and manufacturer’s declaration – electromagnetic immunity			
The TruNode Gamma Probe System is intended for use in the electromagnetic environment specified below. The customer or the user of the TruNode Gamma Probe System should assure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment – guidance
Conducted RF IEC 61000-4-6	3 Vrms 150 kHz to 80 MHz (6 Vrms in ISM radio Bands within 150kHz – 80MHz)	3 Vrms	Portable and mobile RF communications equipment should be used no closer to any part of the TruNode Gamma Probe System, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter. Recommended separation distance $d = 1.2\sqrt{P}$
Radiated RF IEC 61000-4-3	3 V/m 80 MHz to 2.7 GHz	3 V/m	$d = 1.2\sqrt{P}$ 80 MHz to 800 MHz $d = 2.3\sqrt{P}$ 800 MHz to 2.7 GHz where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters (m). Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey ^a , should be less than the compliance level in each frequency range. ^b
NOTE 1 At 80 MHz and 800 MHz, the higher frequency range applies. NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.			

^a Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the TruNode Gamma Probe System is used exceeds the applicable RF compliance level above, the TruNode Gamma Probe System should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the TruNode Gamma Probe System.

^b Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

Recommended separation distances between portable and mobile RF communications equipment and the TruNode Gamma Probe System

The TruNode Gamma Probe System is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the TruNode Gamma Probe System can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the TruNode Gamma Probe System as recommended below, according to the maximum output power of the communications equipment.

Rated maximum output power of transmitter W	Separation distance according to frequency of transmitter m		
	150 kHz to 80 MHz $d = 1.2\sqrt{P}$	80 MHz to 800 MHz $d = 1.2\sqrt{P}$	800 MHz to 2.7 GHz $d = 2.3\sqrt{P}$
0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance d in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE 1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

Immunity to RF Wireless Communications Equipment						
Test Frequency (MHz)	Band ^{a)} (MHz)	Service ^{a)}	Modulation ^{b)}	Max Power (W)	Distance (m)	IMMUNITY TEST LEVEL (V/m)
385	380 – 390	TETRA 400	Pulse modulation ^{b)} 18 Hz	1.8	0.3	27
450	430 – 470	GMRS 460, FRS 460	FM ^{c)} ± 5 kHz deviation 1 kHz sine	2	0.3	28
710	704 – 787	LTE Band 13, 17	Pulse modulation ^{b)} 217 Hz	0.2	0.3	9
745						
780						
810	800 – 960	GSM 800/900, TETRA 800, iDEN 820, CDMA 850, LTE Band 5	Pulse modulation ^{b)} 18 Hz	2	0.3	28
870						
930						
1720	1 700 – 1 990	GSM 1800; CDMA 1900; GSM 1900; DECT; LTE Band 1, 3, 4, 25; UMTS	Pulse modulation ^{b)} 217 Hz	2	0.3	28
1845						
1970						
2450	2 400 – 2 570	Bluetooth, WLAN, 802.11 b/g/n, RFID 2450, LTE Band 7	Pulse modulation ^{b)} 217 Hz	2	0.3	28
5240	5 100 – 5 800	WLAN 802.11 a/n	Pulse modulation ^{b)} 217 Hz	0.2	0.3	9
5500						
5785						
a) For some services, only the uplink frequencies are included. b) The carrier shall be modulated using a 50 % duty cycle square wave signal. c) As an alternative to FM modulation, 50 % pulse modulation at 18 Hz may be used because while it does not represent actual modulation, it would be worst case.						

13. FCC INFORMATION

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

- FCC Part 15C: Intentional Radiators – FCC IDs
Probe: 2ADNA-S10
UFU with Samsung tablet: ZCASMT-290



Caution: changes or modifications not expressly approved by Hologic Inc. could void the user's authority to operate the equipment.

14. TECHNICAL SUPPORT AND PRODUCT COMPLAINTS

Report any complaints or problems in the quality, reliability, safety, or performance of this product to Hologic. If the device has caused or added to patient injury, immediately report the incident to Hologic Authorized Representative and Competent authority of the respective member state or country. The Competent Authorities, for medical devices, are usually the individual Member States' Ministry of Health, or an agency within the Ministry of Health.

For technical support or reorder information in the United States, please contact:



Hologic, Inc.
250 Campus Drive
Marlborough, MA 01752 USA
Phone: 1-877-371-4372
WWW.hologic.com

International customers, contact your distributor or local Hologic sales representative:



Hologic BV
Da Vincilaan 5
1930 Zaventem
Belgium
Tel: +32 2 711 46 80

REPLACEMENT PARTS

Contact your local Hologic representative to order replacement parts.

The only user replaceable part for the TruNode UFU is the power supply.

Hologic P/N	Description
120-807633	TruNode UFU Power Supply Kit (for 120-807606; provided with USA style plug).
120-807632	TruNode UFU Power Supply Kit (for 120-807611; provided with UK, EU, and AU style interchangeable plugs).



Caution: Only use power supplies and interchangeable plugs approved by Hologic. Use of any other power supplies and interchangeable plugs may damage the TruNode UFU and void your warranty.

15. QUALITY ASSURANCE TESTING

Local regulations may require a series of tests be performed in specified time intervals to ensure that the functional performance of the equipment meets established criteria. If constancy testing is required, please refer the following link to access the testing procedure for the TruNode Probes:

<https://www.hologic.com/package-inserts>.

16. REPLACING THE POWER SUPPLY INTERCHANGEABLE PLUG


There are four interchangeable plugs available for the TruNode UFU power supply. These interchangeable plugs are configured for the following regions: United States and Canada (USA Style), European Union (EU Style), United Kingdom (UK Style), and Australia (AU Style). The power supply is universal and will work in each of the above regions simply by installing the proper interchangeable plug.

NOTES:


- The TruNode UFUs power supply ships in one of two configurations:
 - With a USA style interchangeable plug (for the United States and Canada), or
 - With EU, UK, and AU style interchangeable plugs.
- The power supply ships without a plug installed. Install the appropriate plug per the following instructions before using the power supply.
- The following instructions show the installation of the USA Style Interchangeable Plug, but the steps are identical for all plug styles.

1. Installing the interchangeable plug: (refer to figures below)

- A. Align the tabs on the interchangeable plug with the slots in the power supply.
- B. Insert the plug into the power supply.
- C. Slide the plug back until it locks into place.

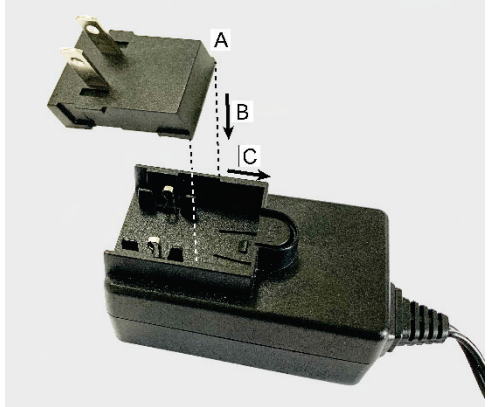


- D. You should not be able to remove the interchangeable plug without pressing the button.
- E. The power supply is now ready for use.

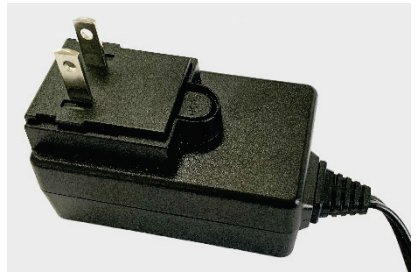

2. Replacing the interchangeable plug: (refer to figure below)

- A. Unplug the power supply from the facilities mains receptacle.
- B. Press the button to unlock the interchangeable plug.
- C. Slide the plug forward (away from the button) ~13mm (0.5").
- D. Lift the interchangeable plug out of the power supply.
- E. Follow 1 above to install a new plug.

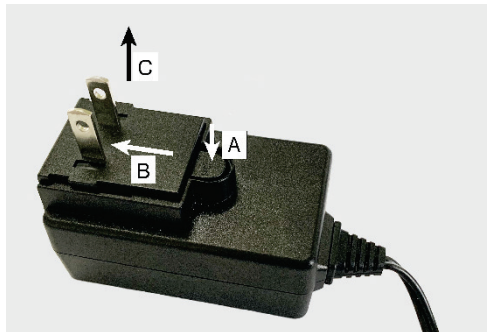

This page is intentionally left blank