

# Actim<sup>®</sup> PROM

A qualitative test for the detection of amniotic fluid in vaginal secretions.



- ▶ Identifies IGFBP-1 in vaginal swab specimens.<sup>1</sup>
- ▶ Remains effective in the presence of vaginal bleeding and other common contaminants.\*<sup>1</sup>
- ▶ Results available in 5 minutes or less.<sup>1</sup>



Now the Exclusive  
**U.S. Distributor**



Scan to discover  
more information

# Actim<sup>®</sup> PROM

## Test Kit Technical Specifications<sup>1</sup>

<b>Test Principle</b>	Qualitative immunochromatographic test
<b>Target Protein</b>	IGFBP-1 (insulin-like growth factor binding protein-1)
<b>Specimen Type</b>	Vaginal secretions
<b>Specimen Collection</b>	Swab specimen from posterior fornix with or without a speculum
<b>Reading Time</b>	5 minutes
<b>Interpretation</b>	Visual
<b>Cut-off</b>	25 ug/L in the extracted specimen
<b>Sensitivity</b>	95.5% (with speculum) 90.1% (without speculum)
<b>Specificity</b>	86.4% (with speculum) 91.0% (without speculum)
<b>Test Kit Components</b>	Each test contains 1 swab, 1 tube of Specimen Extraction Solution, 1 dipstick
<b>Control Kit Components</b>	1 negative control, 1 low positive control, 1 high positive control, 1 reconstitution solution

## Ordering Information

Product	Part Number	Storage Conditions <sup>1,2</sup>
Actim PROM 10-Test Kit	30831ETUS	2°C – 25°C (36°F – 77°F)
Actim PROM Controls	30800ETUS	2°C – 25°C (36°F – 77°F)

[hologic.com](http://hologic.com) | [diagnostic.solutions@hologic.com](mailto:diagnostic.solutions@hologic.com) | +1.888.484.4747






\* The test has been designed to minimize interference from bleeding, but in cases of heavy bleeding the blood locally may have a higher concentration of IGFBP-1 protein. In these cases, a positive result should be interpreted with caution.

Hologic provides this collection procedure as a general information tool only; it is not an affirmative instruction or guarantee of performance. It is the sole responsibility of medical professionals to read and understand the appropriate package insert and comply with applicable local, state and federal rules and regulations.

**References:** 1. Actim PROM Test Kit Instructions For Use. A30831ETUS-IFU Rev. C. Hologic, Inc.; 2025. 2. Actim PROM Controls Instructions For Use. A30800ETUS-IFU Rev. C. Hologic, Inc.; 2025.

MISC-10803-001 Rev. 002 © 2025 Hologic, Inc. All rights reserved. Hologic and associated logos are trademarks and/or trademarks of Hologic, Inc. and/or its subsidiaries in the United States and/or other countries. Certain images, text, and related content displayed on this webpage is used with the permission of Actim Oy. Actim<sup>®</sup> is a registered trademark of Actim Oy. All other trademarks that may appear are the property of their respective owners.

## Test Procedure

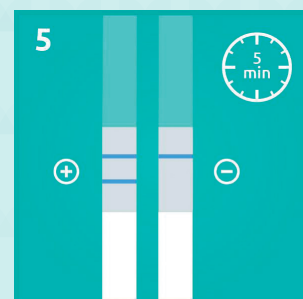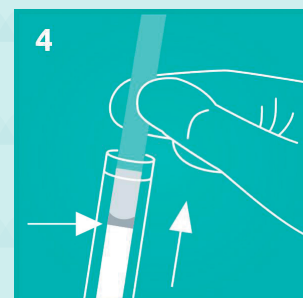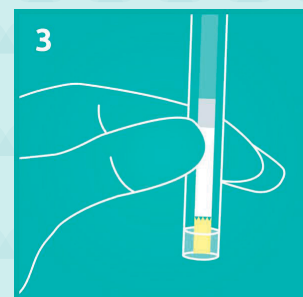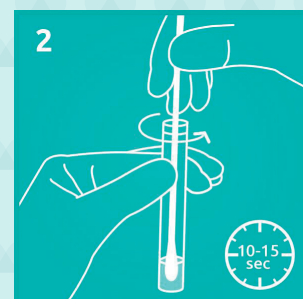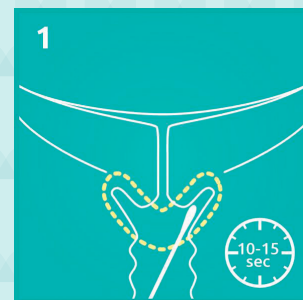

⊕ **Positive results** can be read as soon as they become visible.<sup>1</sup>

⊖ **Negative results** should be confirmed at 5 minutes.<sup>1</sup>